

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
 Data File : PD073043.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2022 04:47
 Operator : AR\AJ
 Sample : INDB401
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 05:41:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 05:39:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.698	3.459	94763268	2548.8E6	38.128	36.474
27)	SA Decachlor...	7.828	8.913	179.3E6	1153.6E6	71.954	71.359
Target Compounds							
5)	MB Aldrin	4.143	5.162	136.4E6	1476.4E6	40.554	33.998
6)	B beta-BHC	3.833	4.472	60702156	976.2E6	35.832	33.551
7)	B delta-BHC	4.063	4.716	149.7E6	2020.0E6	42.048	34.703
8)	B Heptachlo...	4.648	5.595	123.3E6	1250.8E6	39.077	34.418
10)	B trans-Chl...	4.896	5.848	122.4E6	1190.9E6	39.237	35.554
11)	B cis-Chlor...	4.959	5.923	123.6E6	1202.8E6	38.777	35.717
12)	B 4,4'-DDE	5.148	6.097	246.7E6	2299.0E6	83.752	73.232
15)	B Endosulfa...	5.857	6.717	214.7E6	1846.7E6	78.569	72.758
18)	B Endrin al...	6.039	6.849	168.5E6	1434.3E6	75.553	71.396
19)	B Endosulfa...	6.263	7.081	199.0E6	1592.2E6	77.780	73.081
21)	B Endrin ke...	6.773	7.571	230.5E6	1698.4E6	77.305	72.227

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
Data File : PD073043.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2022 04:47
Operator : AR\AJ
Sample : INDB401
Misc :
ALS Vial : 37 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 05:41:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 05:39:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

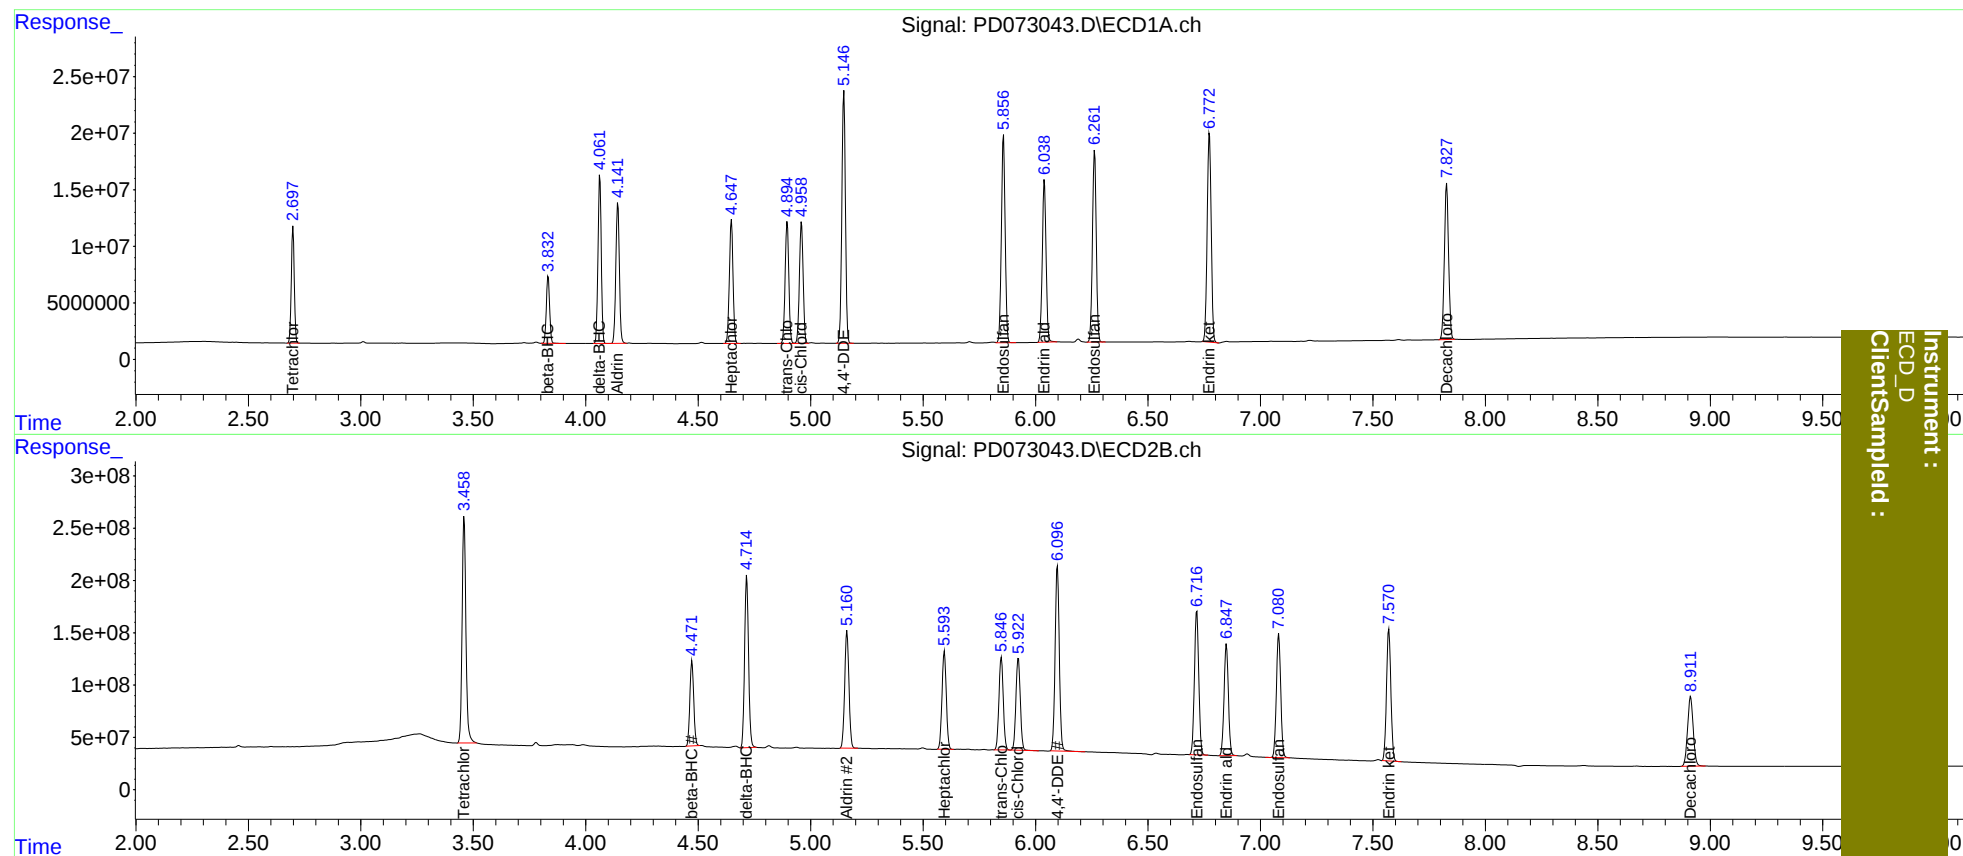


Instrument :
ECD_D
ClientSampled :

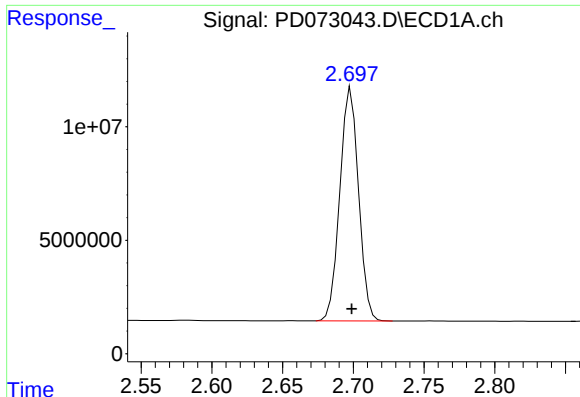

#1 Tetrachloro-m-xylene


R.T.: 2.698 min
Delta R.T.: 0.000 min
Response: 94763268
Conc: 38.13 ng/ml

Instrument :
ECD_D
ClientSampleId :

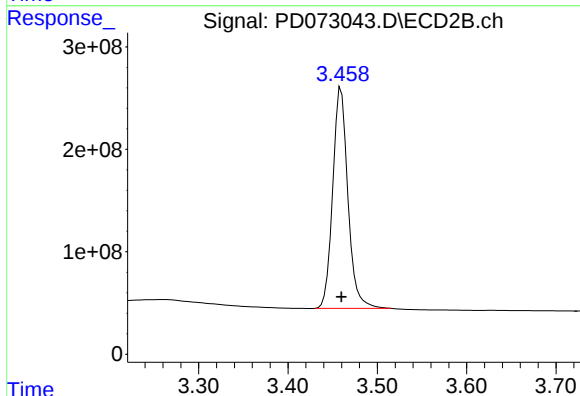


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 2548805508
Conc: 36.47 ng/ml

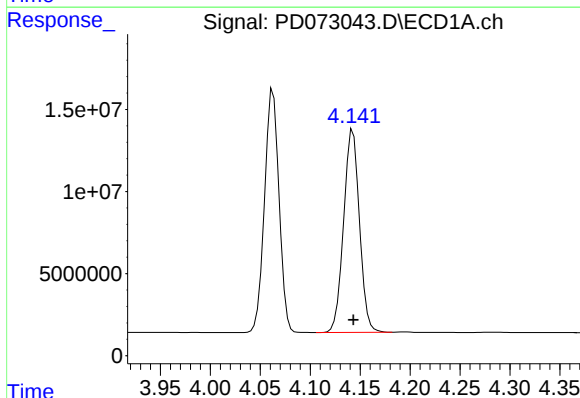


#5 Aldrin

R.T.: 4.143 min
Delta R.T.: 0.000 min
Response: 136408850
Conc: 40.55 ng/ml

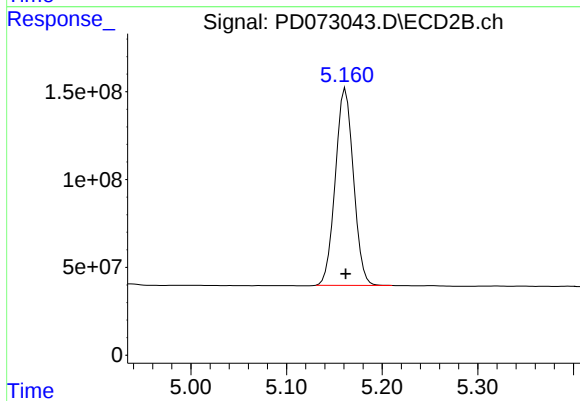

#5 Aldrin


R.T.: 5.162 min
Delta R.T.: 0.000 min
Response: 1476359007
Conc: 34.00 ng/ml

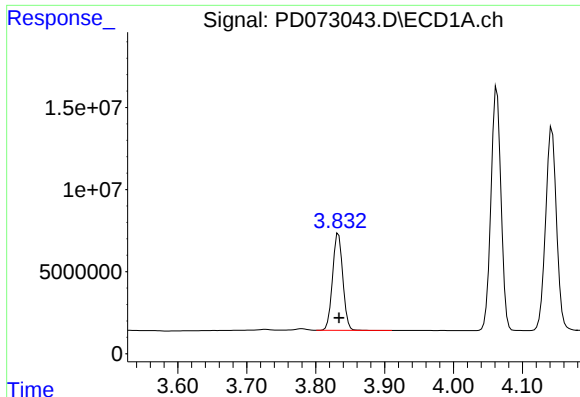

#6 beta-BHC


R.T.: 3.833 min
Delta R.T.: 0.000 min
Response: 60702156
Conc: 35.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

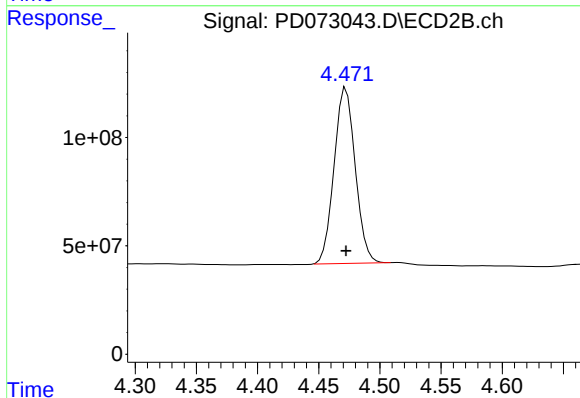


#6 beta-BHC

R.T.: 4.472 min
Delta R.T.: 0.000 min
Response: 976165637
Conc: 33.55 ng/ml

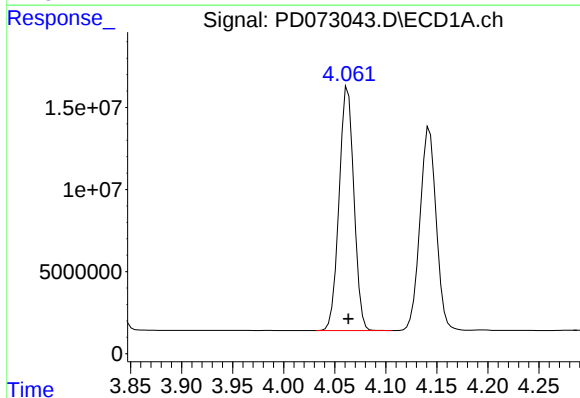


#7 delta-BHC

R.T.: 4.063 min
Delta R.T.: 0.000 min
Response: 149732082
Conc: 42.05 ng/ml

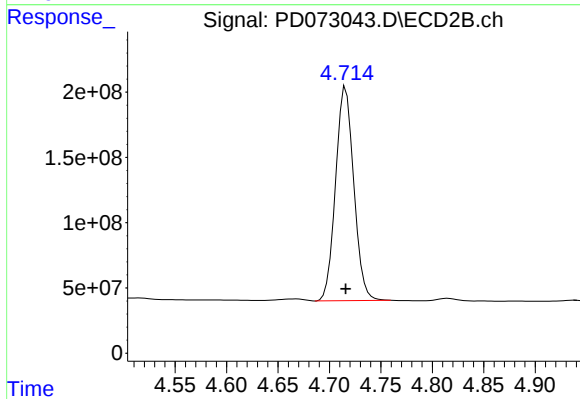

#7 delta-BHC


R.T.: 4.716 min
Delta R.T.: 0.000 min
Response: 2020031930
Conc: 34.70 ng/ml

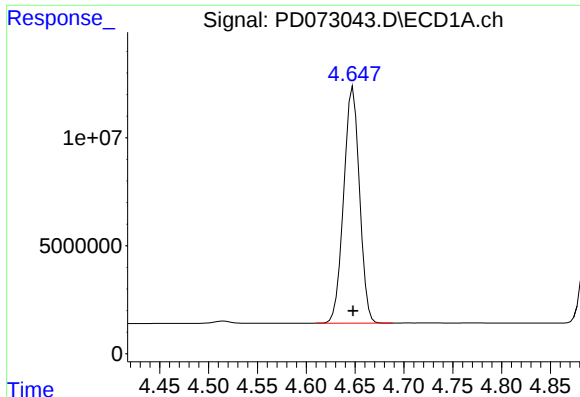

#8 Heptachlor epoxide


R.T.: 4.648 min
Delta R.T.: 0.000 min
Response: 123256781
Conc: 39.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

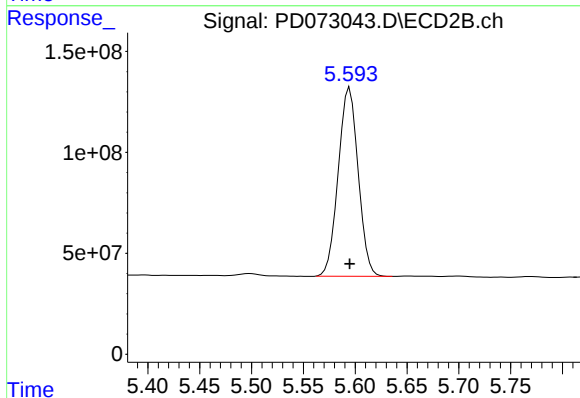


#8 Heptachlor epoxide

R.T.: 5.595 min
Delta R.T.: 0.000 min
Response: 1250842996
Conc: 34.42 ng/ml

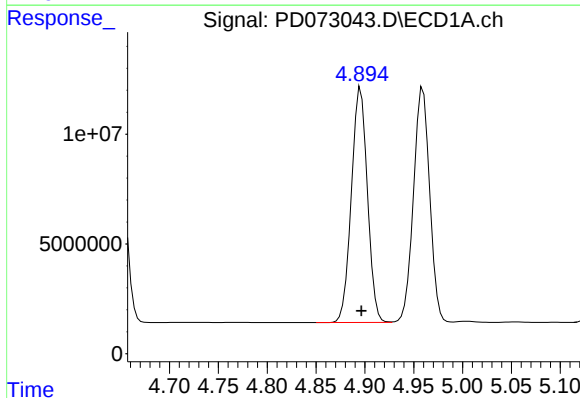


#10 trans-Chlordane

R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 122350133
Conc: 39.24 ng/ml

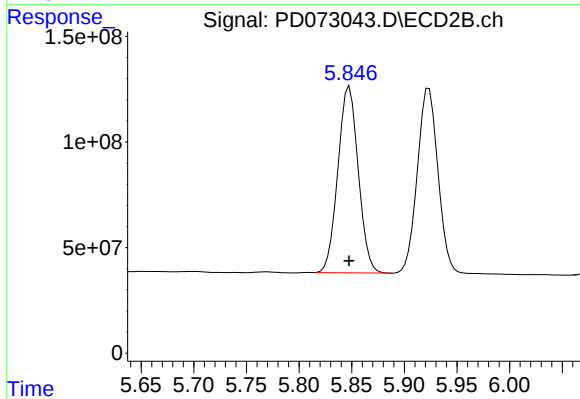

#10 trans-Chlordane


R.T.: 5.848 min
Delta R.T.: 0.000 min
Response: 1190945530
Conc: 35.55 ng/ml

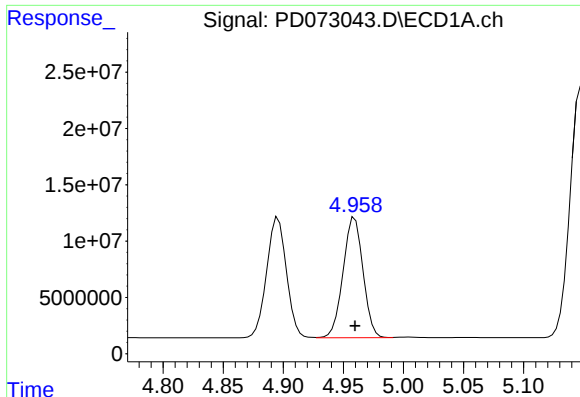

#11 cis-Chlordane


R.T.: 4.959 min
Delta R.T.: 0.000 min
Response: 123649178
Conc: 38.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

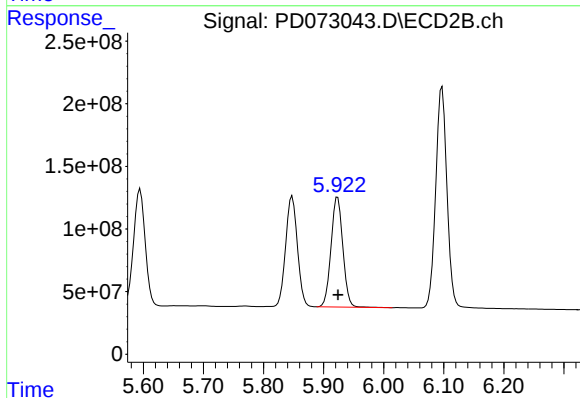


#11 cis-Chlordane

R.T.: 5.923 min
Delta R.T.: 0.000 min
Response: 1202756340
Conc: 35.72 ng/ml

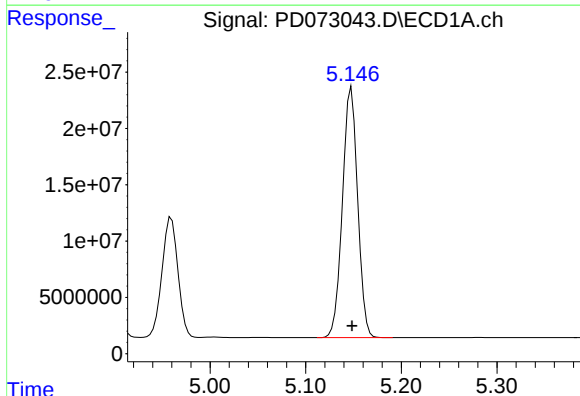


#12 4,4'-DDE

R.T.: 5.148 min
Delta R.T.: 0.000 min
Response: 246686942
Conc: 83.75 ng/ml

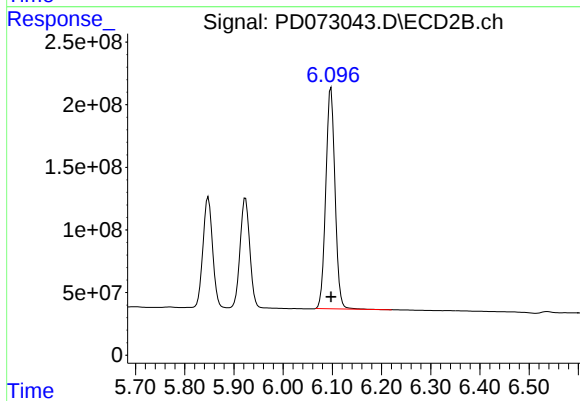

#12 4,4'-DDE


R.T.: 6.097 min
Delta R.T.: 0.000 min
Response: 2299041118
Conc: 73.23 ng/ml

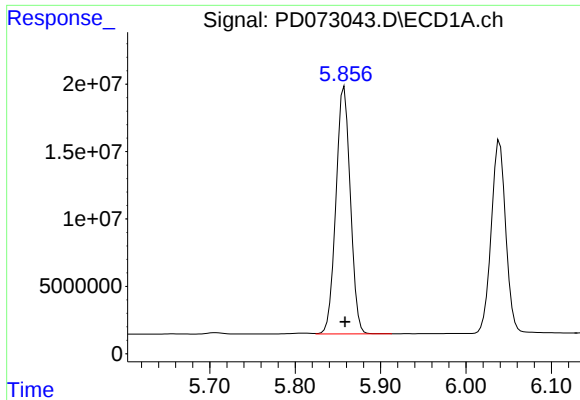

#15 Endosulfan II


R.T.: 5.857 min
Delta R.T.: 0.000 min
Response: 214651788
Conc: 78.57 ng/ml

Instrument :
ECD_D
ClientSampleId :

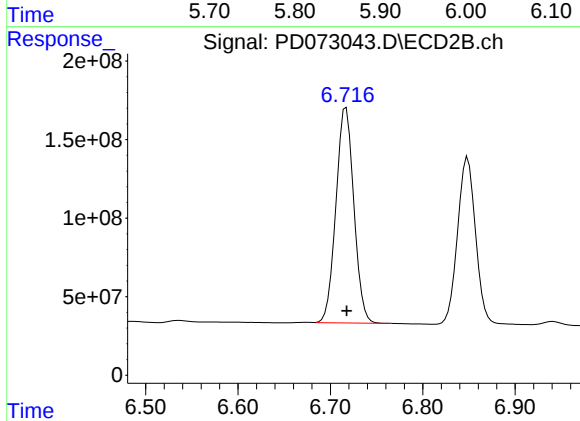


#15 Endosulfan II

R.T.: 6.717 min
Delta R.T.: 0.000 min
Response: 1846705306
Conc: 72.76 ng/ml

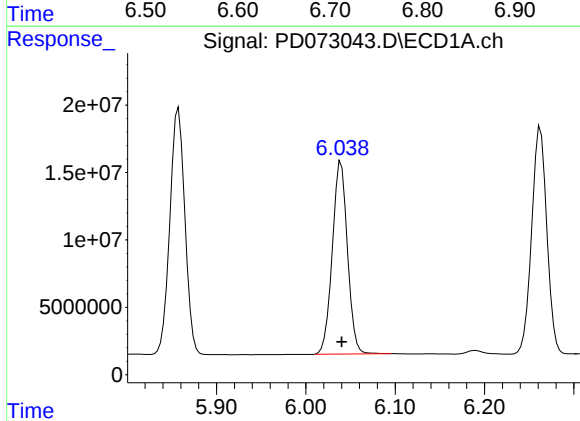


#18 Endrin aldehyde

R.T.: 6.039 min
Delta R.T.: 0.000 min
Response: 168453671
Conc: 75.55 ng/ml

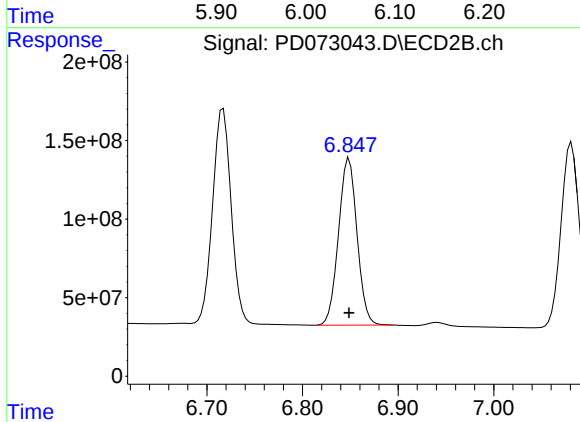

#18 Endrin aldehyde


R.T.: 6.849 min
Delta R.T.: 0.000 min
Response: 1434286500
Conc: 71.40 ng/ml

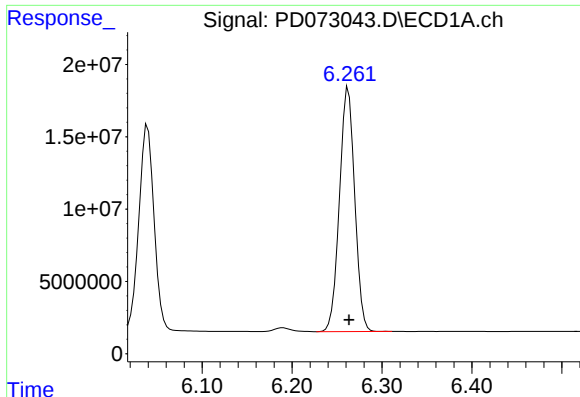

#19 Endosulfan Sulfate


R.T.: 6.263 min
Delta R.T.: 0.000 min
Response: 198953932
Conc: 77.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

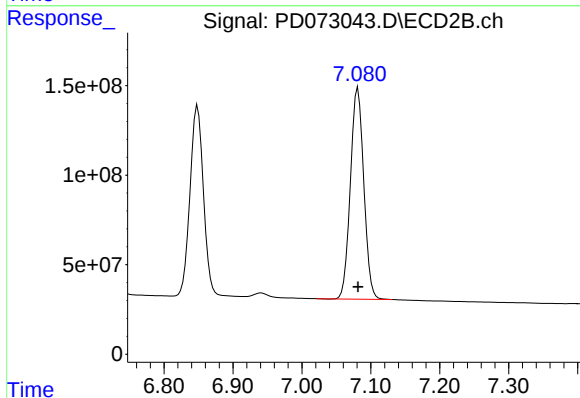


#19 Endosulfan Sulfate

R.T.: 7.081 min
Delta R.T.: 0.000 min
Response: 1592224986
Conc: 73.08 ng/ml

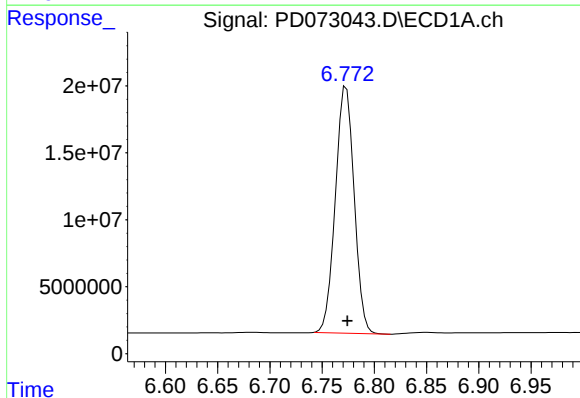


#21 Endrin ketone

R.T.: 6.773 min
Delta R.T.: -0.001 min
Response: 230484544
Conc: 77.30 ng/ml

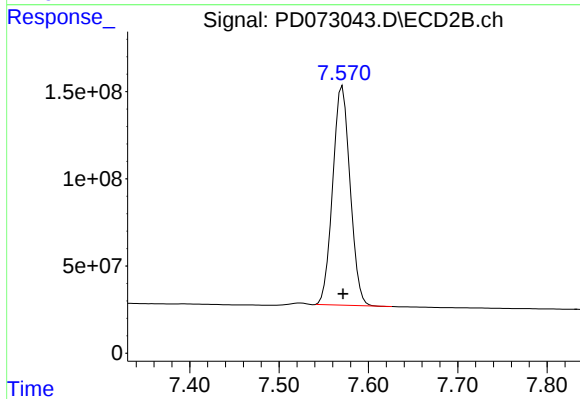

#21 Endrin ketone


R.T.: 7.571 min
Delta R.T.: 0.000 min
Response: 1698447348
Conc: 72.23 ng/ml

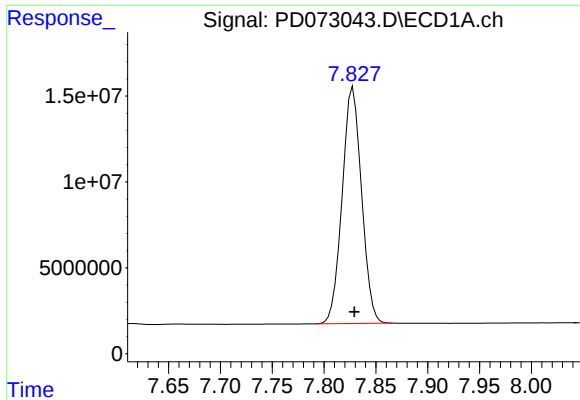

#27 Decachlorobiphenyl

R.T.: 7.828 min
Delta R.T.: -0.001 min
Response: 179317278
Conc: 71.95 ng/ml

Instrument :
ECD_D
ClientSampleId :

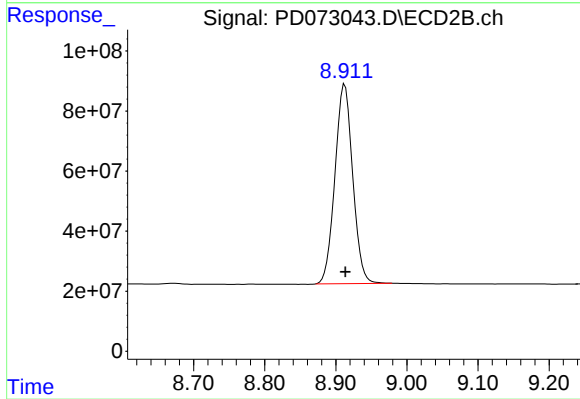

#27 Decachlorobiphenyl

R.T.: 8.913 min
Delta R.T.: 0.000 min
Response: 1153593824
Conc: 71.36 ng/ml