

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
 Data File : PD073044.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2022 05:01
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 06:03:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 05:58:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.699	3.460	186.5E6	4872.8E6	77.953	74.960
27)	SA Decachlor...	7.829	8.913	332.7E6	2123.9E6	147.154	143.294
Target Compounds							
2)	A alpha-BHC	3.202	3.924	316.1E6	6533.3E6	86.291	76.111
3)	MA gamma-BHC...	3.532	4.258	281.0E6	4921.8E6	84.993	73.833
4)	MA Heptachlor	3.864	4.824	272.8E6	3178.8E6	82.466	69.975
9)	A Endosulfan I	5.017	5.979	223.0E6	2072.1E6	79.219	71.336
13)	MA Dieldrin	5.284	6.257	505.7E6	4468.5E6	164.803	148.923
14)	MA Endrin	5.560	6.488	437.9E6	3580.0E6	162.334	146.481
16)	A 4,4'-DDD	5.707	6.622	395.9E6	3375.1E6	163.700	147.819
17)	MA 4,4'-DDT	5.956	6.930	390.5E6	3279.4E6	175.130	153.338
20)	A Methoxychlor	6.539	7.410	961.2E6	6647.4E6	760.901	709.527


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
Data File : PD073044.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2022 05:01
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 38 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 06:03:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 05:58:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

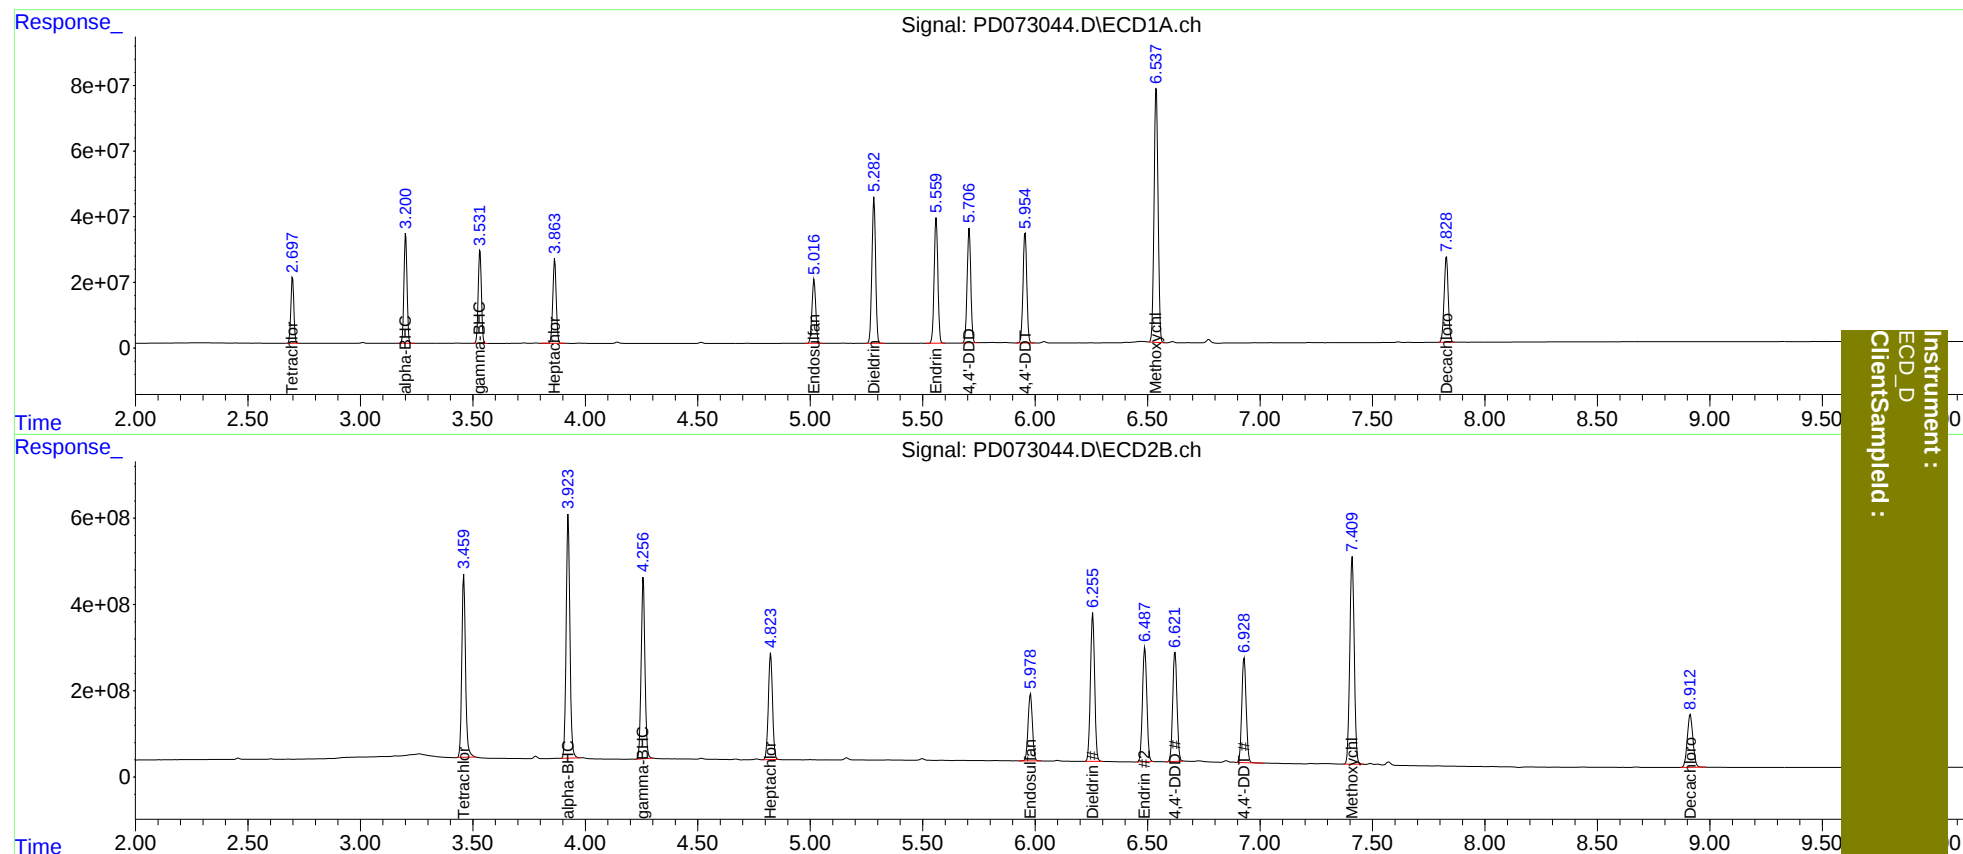


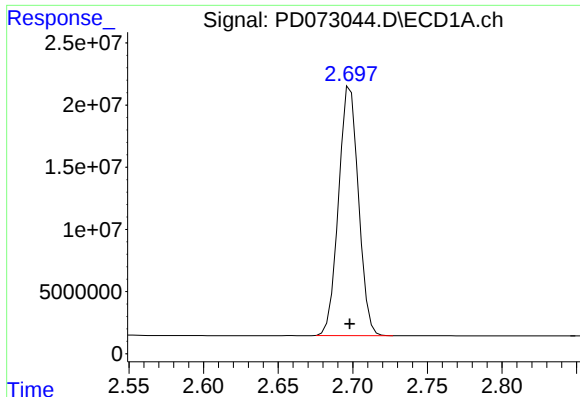

#1 Tetrachloro-m-xylene


R.T.: 2.699 min
Delta R.T.: 0.000 min
Response: 186526368
Conc: 77.95 ng/ml

Instrument :
ECD_D
ClientSampleId :

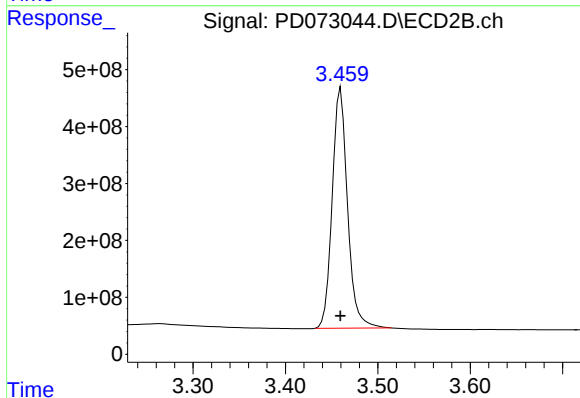


#1 Tetrachloro-m-xylene

R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 4872819834
Conc: 74.96 ng/ml

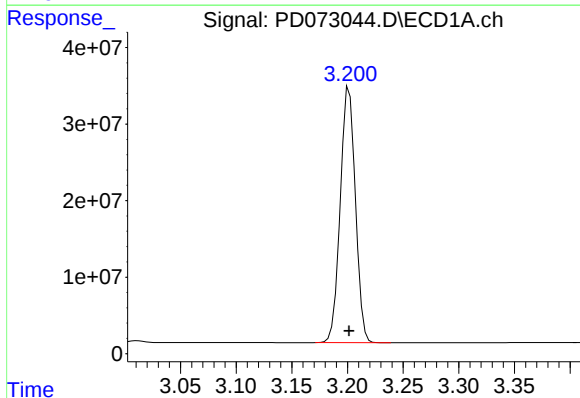


#2 alpha-BHC

R.T.: 3.202 min
Delta R.T.: 0.000 min
Response: 316095067
Conc: 86.29 ng/ml

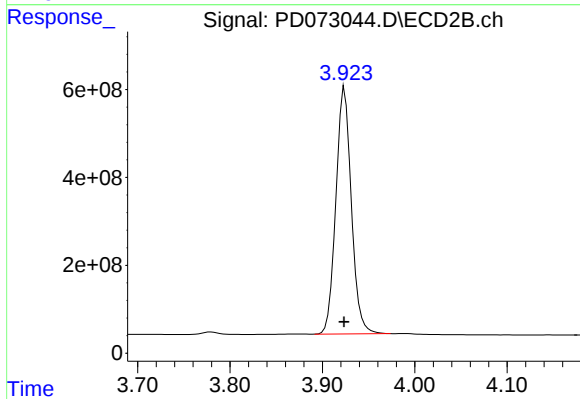

#2 alpha-BHC


R.T.: 3.924 min
Delta R.T.: 0.000 min
Response: 6533292727
Conc: 76.11 ng/ml

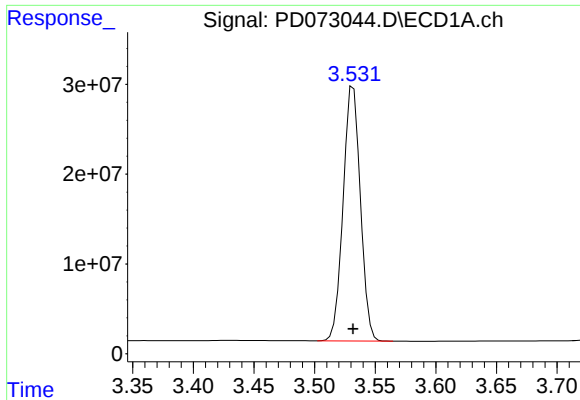

#3 gamma-BHC (Lindane)


R.T.: 3.532 min
Delta R.T.: 0.000 min
Response: 280963238
Conc: 84.99 ng/ml

Instrument :
ECD_D
ClientSampleId :

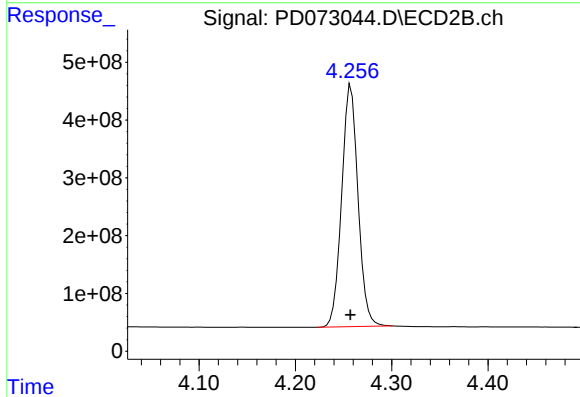


#3 gamma-BHC (Lindane)

R.T.: 4.258 min
Delta R.T.: 0.000 min
Response: 4921808492
Conc: 73.83 ng/ml

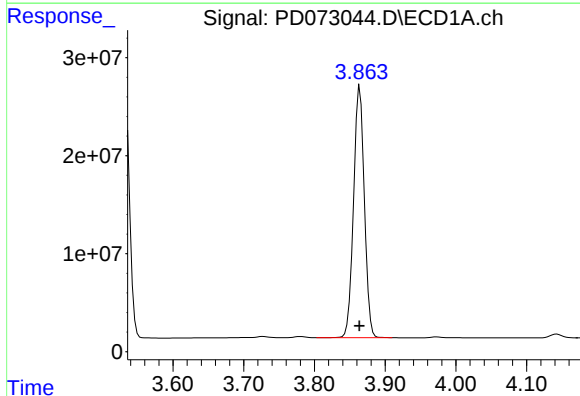


#4 Heptachlor

R.T.: 3.864 min
Delta R.T.: 0.000 min
Response: 272799739
Conc: 82.47 ng/ml

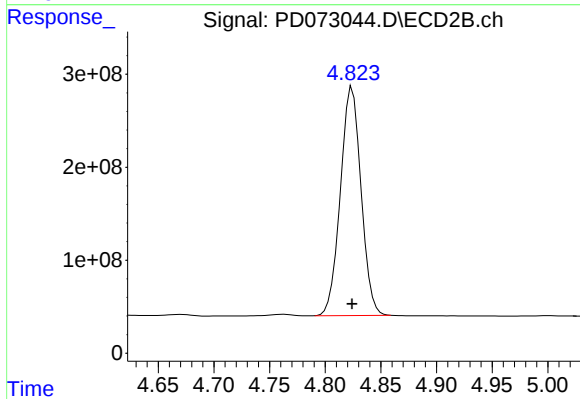

#4 Heptachlor


R.T.: 4.824 min
Delta R.T.: 0.000 min
Response: 3178786939
Conc: 69.97 ng/ml

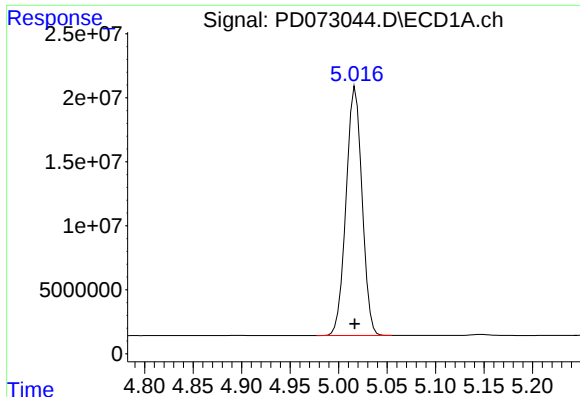

#9 Endosulfan I


R.T.: 5.017 min
Delta R.T.: 0.000 min
Response: 223008248
Conc: 79.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

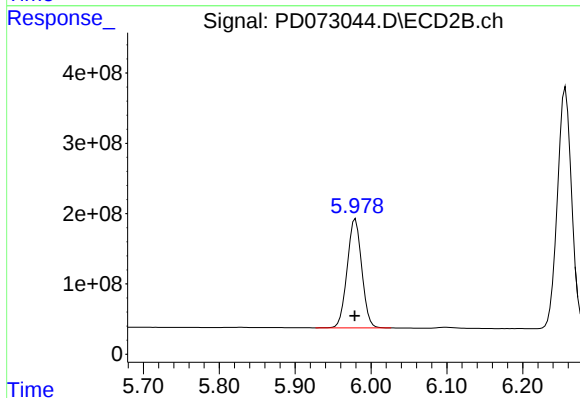


#9 Endosulfan I

R.T.: 5.979 min
Delta R.T.: 0.000 min
Response: 2072099803
Conc: 71.34 ng/ml

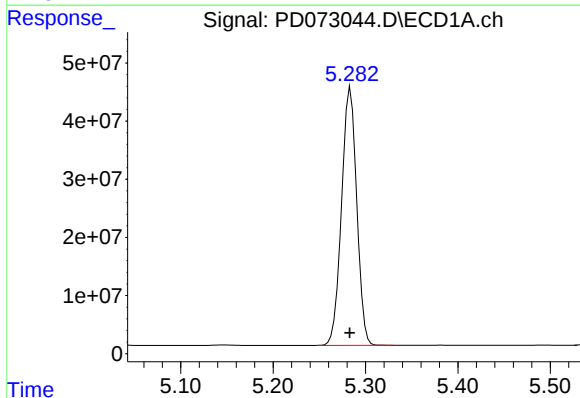


#13 Dieldrin

R.T.: 5.284 min
Delta R.T.: 0.000 min
Response: 505684808
Conc: 164.80 ng/ml

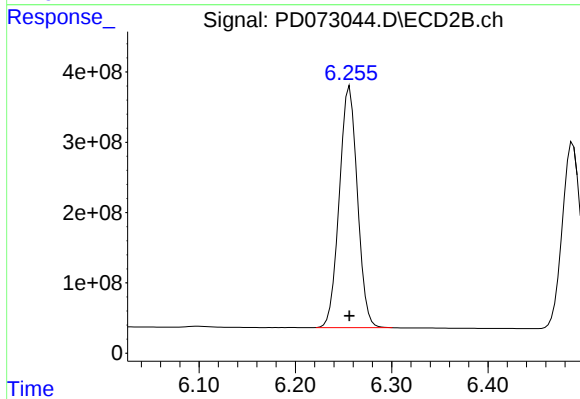

#13 Dieldrin


R.T.: 6.257 min
Delta R.T.: 0.000 min
Response: 4468489880
Conc: 148.92 ng/ml

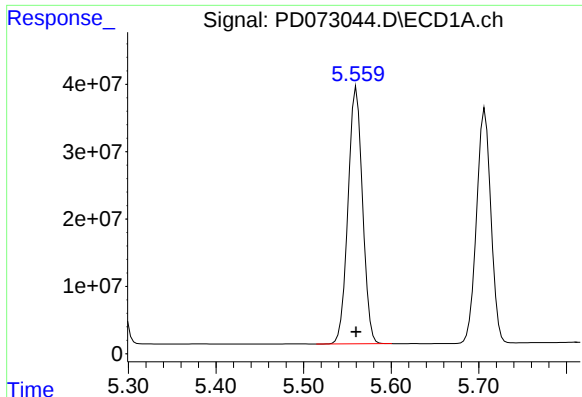

#14 Endrin


R.T.: 5.560 min
Delta R.T.: 0.000 min
Response: 437936093
Conc: 162.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

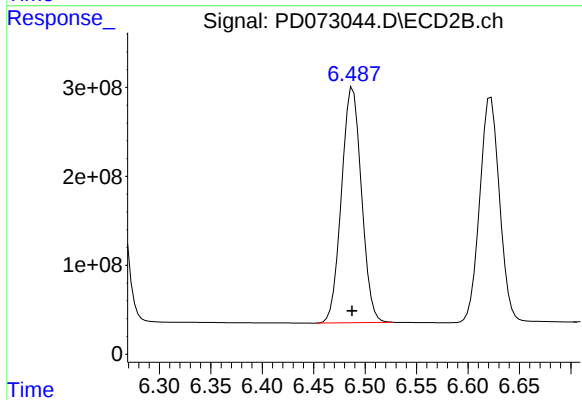


#14 Endrin

R.T.: 6.488 min
Delta R.T.: 0.000 min
Response: 3580015889
Conc: 146.48 ng/ml

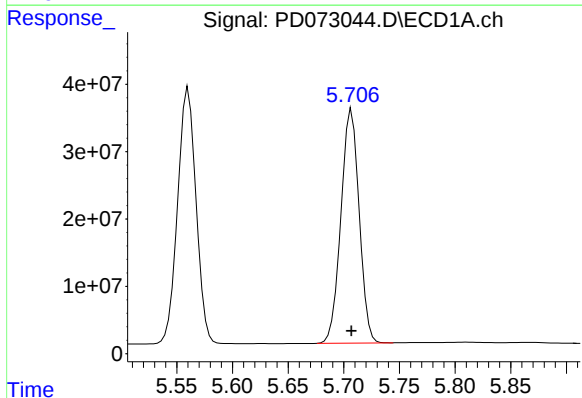


#16 4,4'-DDD

R.T.: 5.707 min
Delta R.T.: 0.000 min
Response: 395919432
Conc: 163.70 ng/ml

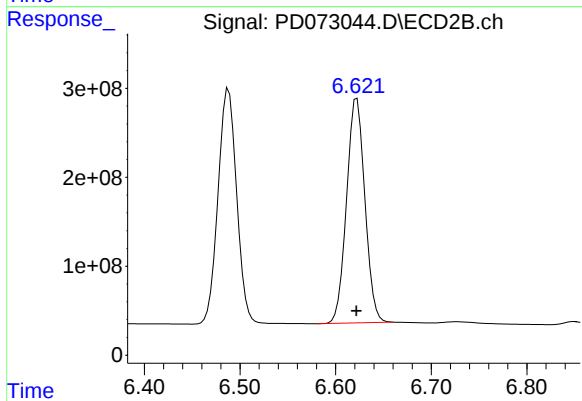

#16 4,4'-DDD


R.T.: 6.622 min
Delta R.T.: 0.000 min
Response: 3375142038
Conc: 147.82 ng/ml

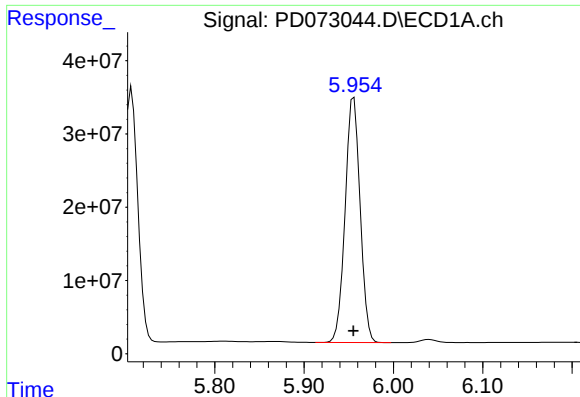

#17 4,4'-DDT


R.T.: 5.956 min
Delta R.T.: 0.000 min
Response: 390463911
Conc: 175.13 ng/ml

Instrument :
ECD_D
ClientSampleId :

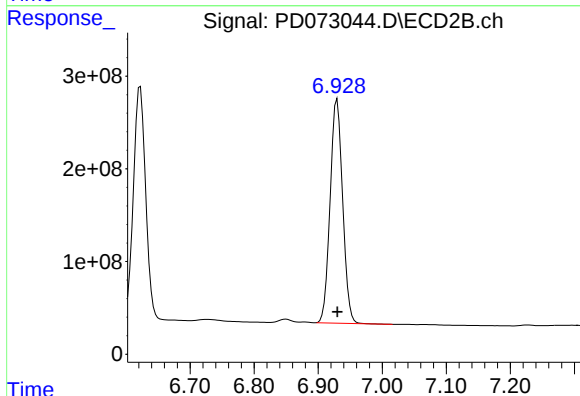


#17 4,4'-DDT

R.T.: 6.930 min
Delta R.T.: 0.000 min
Response: 3279426122
Conc: 153.34 ng/ml

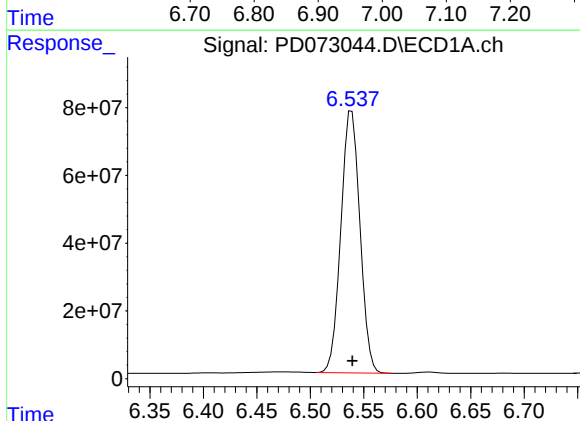


#20 Methoxychlor

R.T.: 6.539 min
Delta R.T.: 0.000 min
Response: 961160306
Conc: 760.90 ng/ml

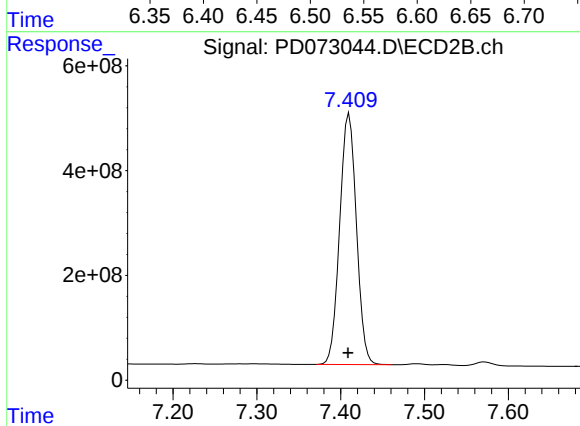

#20 Methoxychlor


R.T.: 7.410 min
Delta R.T.: 0.001 min
Response: 6647449559
Conc: 709.53 ng/ml

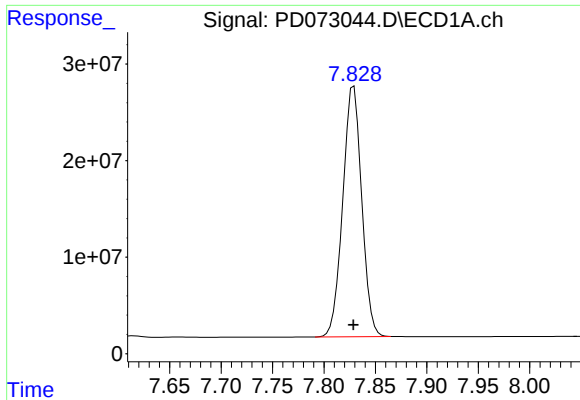

#27 Decachlorobiphenyl

R.T.: 7.829 min
Delta R.T.: 0.000 min
Response: 332717368
Conc: 147.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

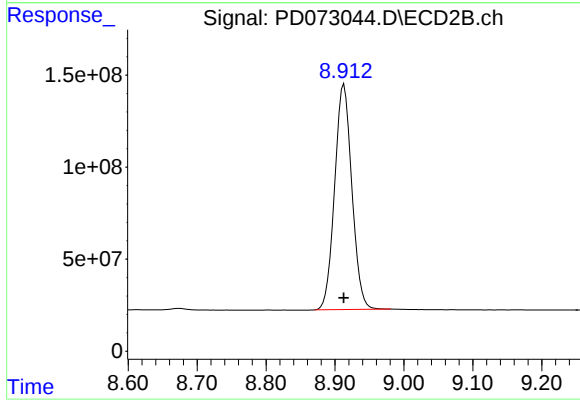

#27 Decachlorobiphenyl

R.T.: 8.913 min
Delta R.T.: 0.000 min
Response: 2123862542
Conc: 143.29 ng/ml