

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
 Data File : PD073029.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2022 01:41
 Operator : AR\AJ
 Sample : RESC42
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC045

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 06:31:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.699	3.459	48973749	1340.3E6	20.423	20.517
2)	SA Decachlor...	7.829	8.913	91333732	589.5E6	40.026	39.833
Target Compounds							
2)	A alpha-BHC	3.202	3.923	35845636	931.2E6	9.794	10.678
3)	MA gamma-BHC...	3.533	4.257	32438662	725.7E6	9.775	10.695
4)	MA Heptachlor	3.865	4.823	33106782	505.2E6	9.910	11.002
5)	MB Aldrin	4.144	5.162	34048148	435.2E6	10.104	10.837
6)	B beta-BHC	3.834	4.473	16606063	289.1E6	10.343	10.819
7)	B delta-BHC	4.064	4.716	35401491	577.6E6	9.741	10.616
8)	B Heptachlo...	4.648	5.594	31351193	358.7E6	10.090	10.611
9)	A Endosulfan I	5.018	5.979	28774045	312.4E6	10.182	10.740
10)	B trans-Chl...	4.897	5.848	30881617	330.3E6	10.020	10.455
11)	B cis-Chlor...	4.960	5.924	31524622	333.0E6	10.068	10.491
12)	B 4,4'-DDE	5.149	6.098	58464909	622.9E6	19.543	20.746
13)	MA Dieldrin	5.284	6.256	60517961	622.7E6	19.755	20.659
14)	MA Endrin	5.561	6.488	54096768	511.0E6	19.954	20.715
15)	B Endosulfa...	5.859	6.718	54647010	502.8E6	20.292	20.814
16)	A 4,4'-DDD	5.707	6.622	47712630	474.5E6	19.804	20.705
17)	MA 4,4'-DDT	5.956	6.930	42058551	440.5E6	18.802	20.510
18)	B Endrin al...	6.041	6.849	44519323	395.0E6	20.612	20.850
19)	B Endosulfa...	6.263	7.081	50682532	427.3E6	20.200	20.548
20)	A Methoxychlor	6.540	7.409	126.5E6	968.6E6	101.012	103.813
21)	B Endrin ke...	6.774	7.571	61201643	467.1E6	20.966	20.920

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
Data File : PD073029.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2022 01:41
Operator : AR\AJ
Sample : RESC42
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 06:31:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

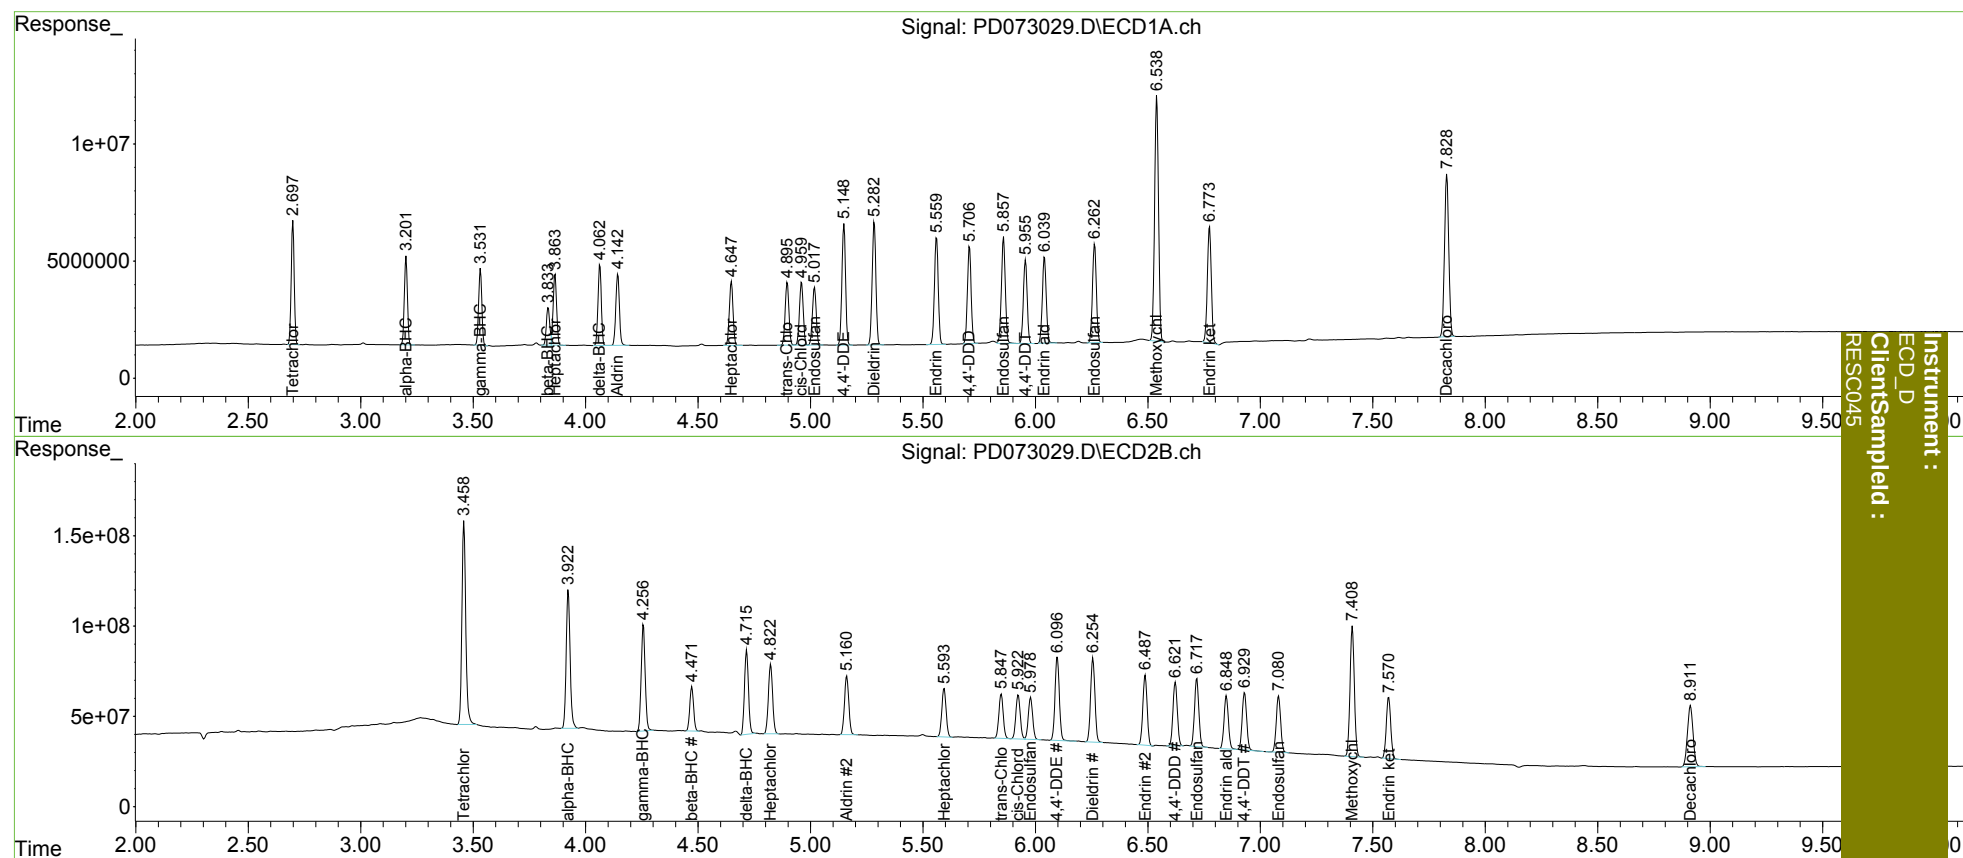

Instrument :
ECD_D
ClientSampled :
RESC045