

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
 Data File : PD073036.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2022 03:14
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA1087

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 06:09:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:09:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.699	3.460	12783946	367.0E6	5.166	5.303
27)	SA Decachlor...	7.829	8.913	25632552	165.6E6	10.626	10.553
Target Compounds							
2)	A alpha-BHC	3.201	3.924	17447636	495.1E6	4.879	5.357
3)	MA gamma-BHC...	3.532	4.258	16181424	393.1E6	4.947	5.412
4)	MA Heptachlor	3.864	4.824	17078694	270.7E6	5.080	5.437
9)	A Endosulfan I	5.017	5.980	14795319	165.9E6	5.125	5.332
13)	MA Dieldrin	5.283	6.257	30306317	332.4E6	9.938	10.511
14)	MA Endrin	5.560	6.489	27643586	279.8E6	10.122	10.675
16)	A 4,4'-DDD	5.707	6.623	23811312	251.9E6	9.922	10.490
17)	MA 4,4'-DDT	5.955	6.931	20922526	229.0E6	9.682	10.343
20)	A Methoxychlor	6.539	7.411	65394953	521.2E6	50.870	52.668

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
Data File : PD073036.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2022 03:14
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 06:09:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:09:31 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

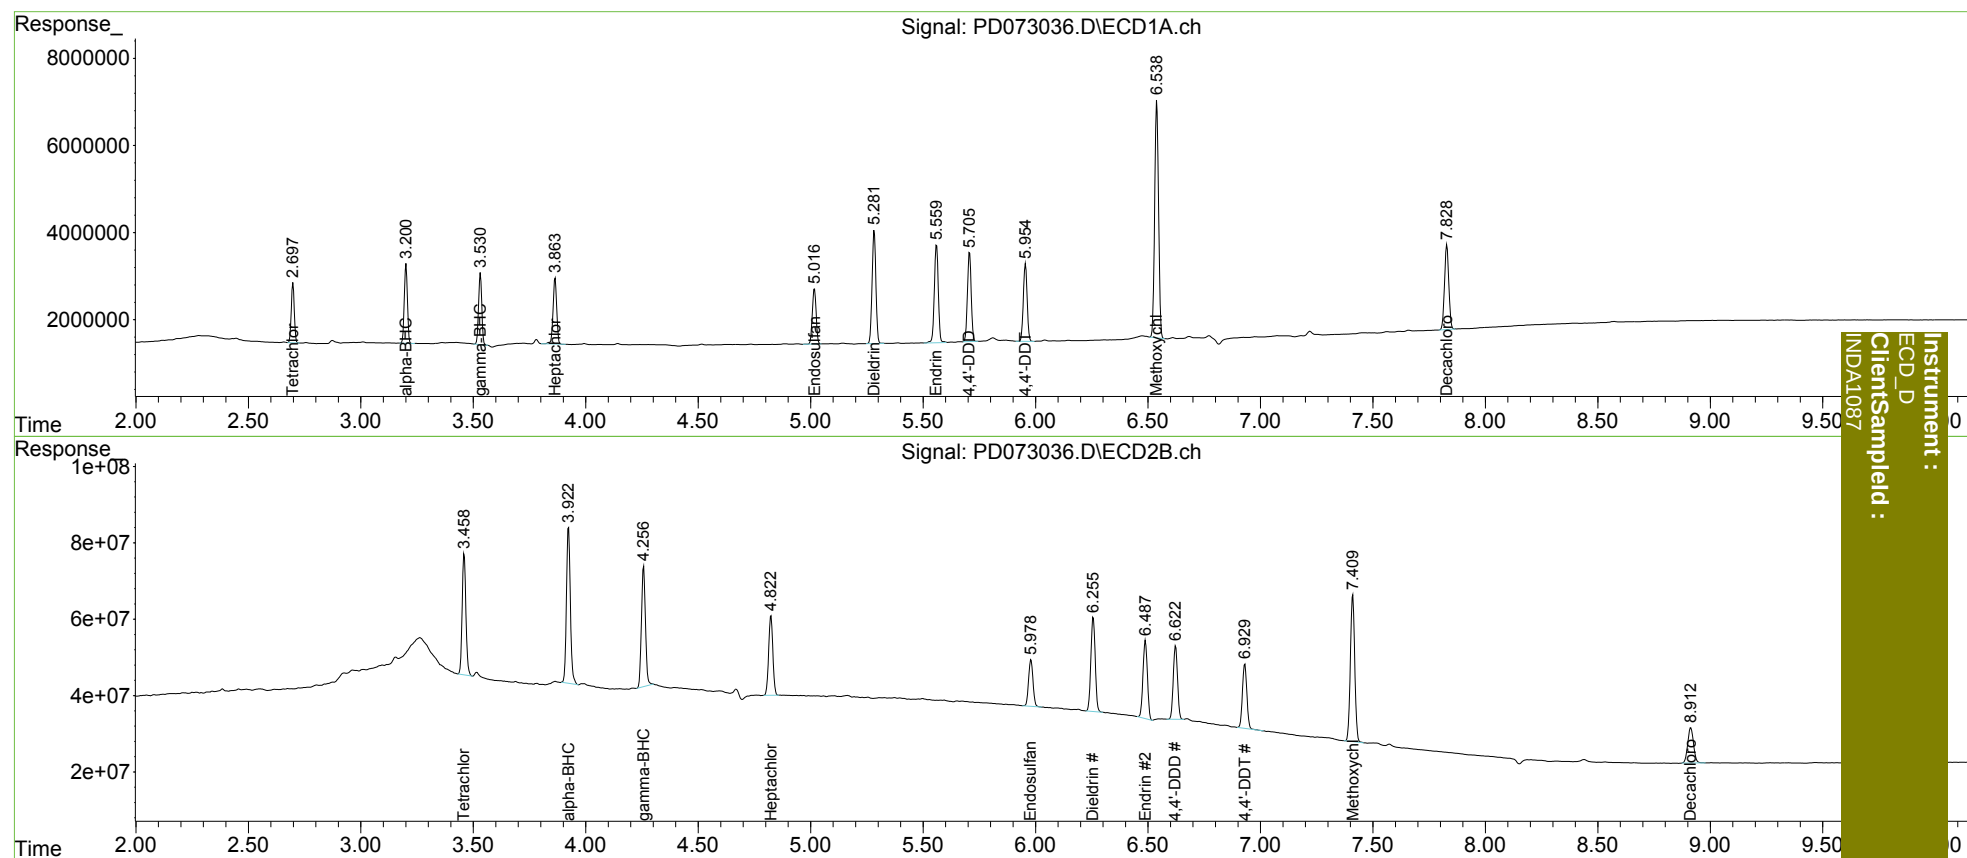

Instrument :
ECD_D
ClientSampled :
INDA1087