

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
 Data File : PD073038.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2022 03:41
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA2089

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 06:11:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:11:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.699	3.459	24093199	673.6E6	9.822	9.820
27)	SA Decachlor...	7.829	8.913	47667399	312.1E6	19.840	19.928
Target Compounds							
2)	A alpha-BHC	3.202	3.923	34773358	899.4E6	9.814	9.819
3)	MA gamma-BHC...	3.532	4.257	32024684	710.3E6	9.859	9.851
4)	MA Heptachlor	3.864	4.823	32731989	490.7E6	9.823	9.905
9)	A Endosulfan I	5.017	5.979	28401878	305.9E6	9.891	9.888
13)	MA Dieldrin	5.283	6.256	59715483	627.5E6	19.719	19.895
14)	MA Endrin	5.560	6.488	53561122	515.2E6	19.740	19.770
16)	A 4,4'-DDD	5.707	6.622	47259212	479.7E6	19.794	19.987
17)	MA 4,4'-DDT	5.956	6.930	42016236	441.9E6	19.626	19.969
20)	A Methoxychlor	6.540	7.410	126.6E6	981.0E6	98.989	99.410

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
Data File : PD073038.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2022 03:41
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 32 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 06:11:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:11:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

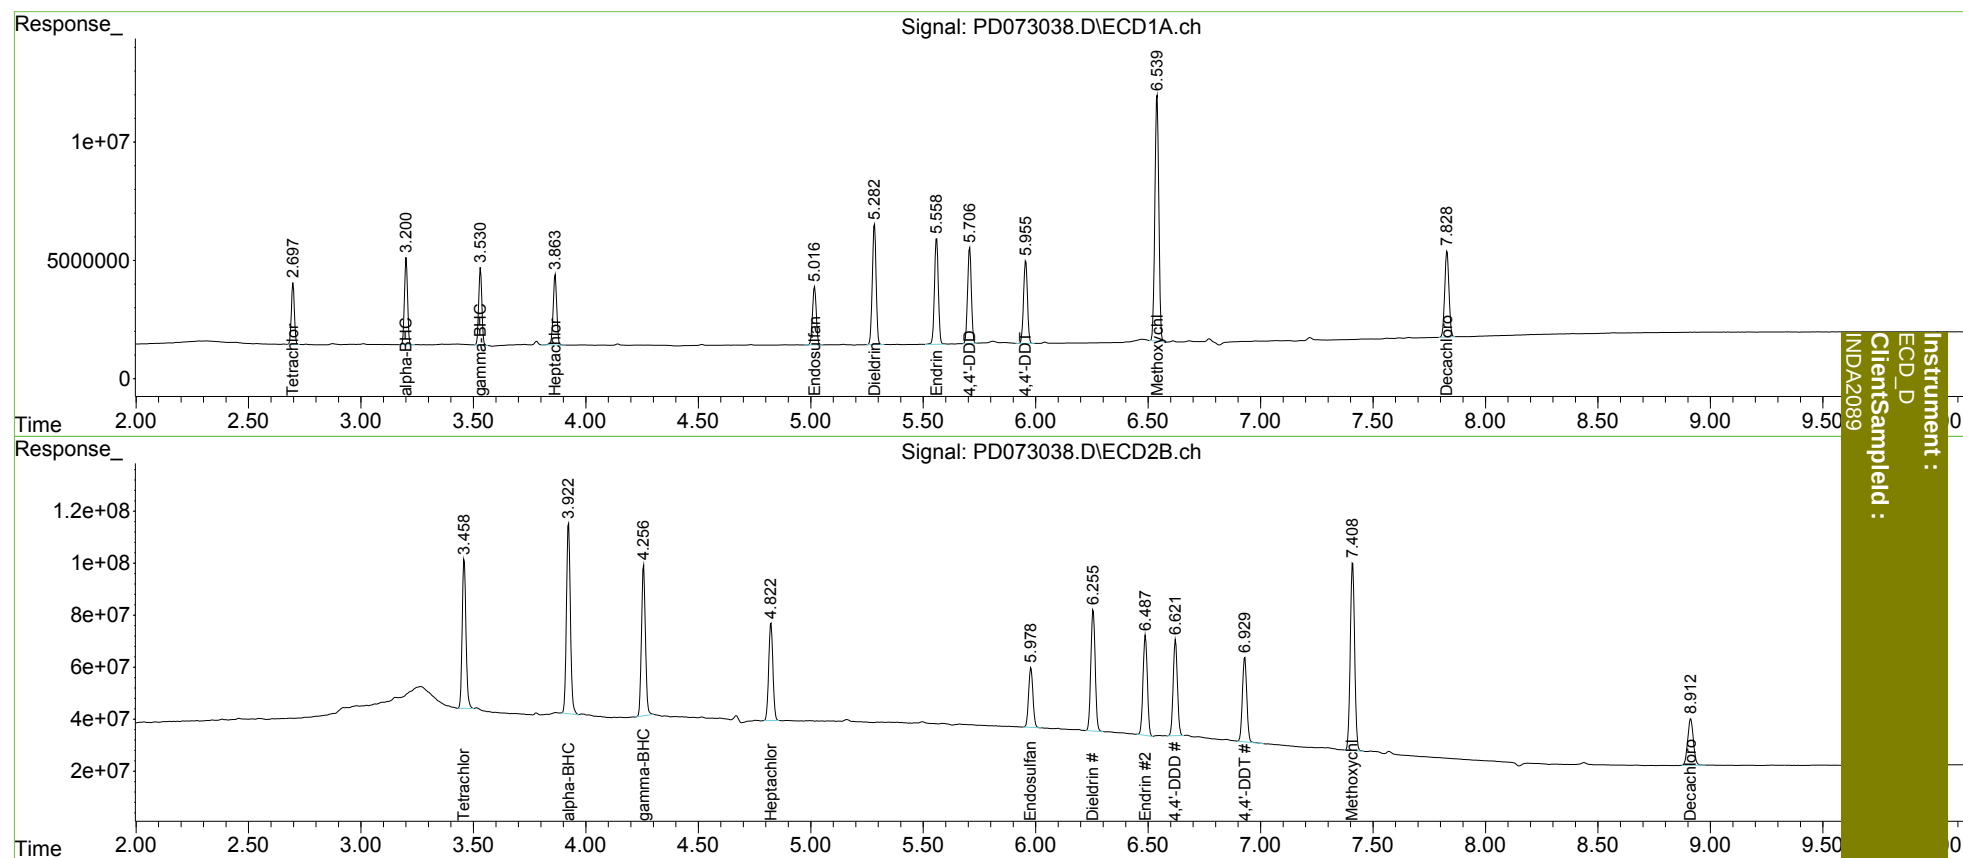

Instrument :
ECD_D
ClientSampled :
INDA2089