

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
 Data File : PD073044.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2022 05:01
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA5095

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 06:15:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:15:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.699	3.460	186.5E6	4872.8E6	77.786	74.594
27)	SA Decachlor...	7.829	8.913	332.7E6	2123.9E6	145.809	143.519
Target Compounds							
2)	A alpha-BHC	3.202	3.924	316.1E6	6533.3E6	86.370	74.918
3)	MA gamma-BHC...	3.532	4.258	281.0E6	4921.8E6	84.661	72.538
4)	MA Heptachlor	3.864	4.824	272.8E6	3178.8E6	81.657	69.223
9)	A Endosulfan I	5.017	5.979	223.0E6	2072.1E6	78.913	71.233
13)	MA Dieldrin	5.284	6.257	505.7E6	4468.5E6	165.071	148.243
14)	MA Endrin	5.560	6.488	437.9E6	3580.0E6	161.539	145.133
16)	A 4,4'-DDD	5.707	6.622	395.9E6	3375.1E6	164.330	147.269
17)	MA 4,4'-DDT	5.956	6.930	390.5E6	3279.4E6	174.552	152.695
20)	A Methoxychlor	6.539	7.410	961.2E6	6647.4E6	767.414	712.446

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
Data File : PD073044.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2022 05:01
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 38 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 06:15:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:15:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

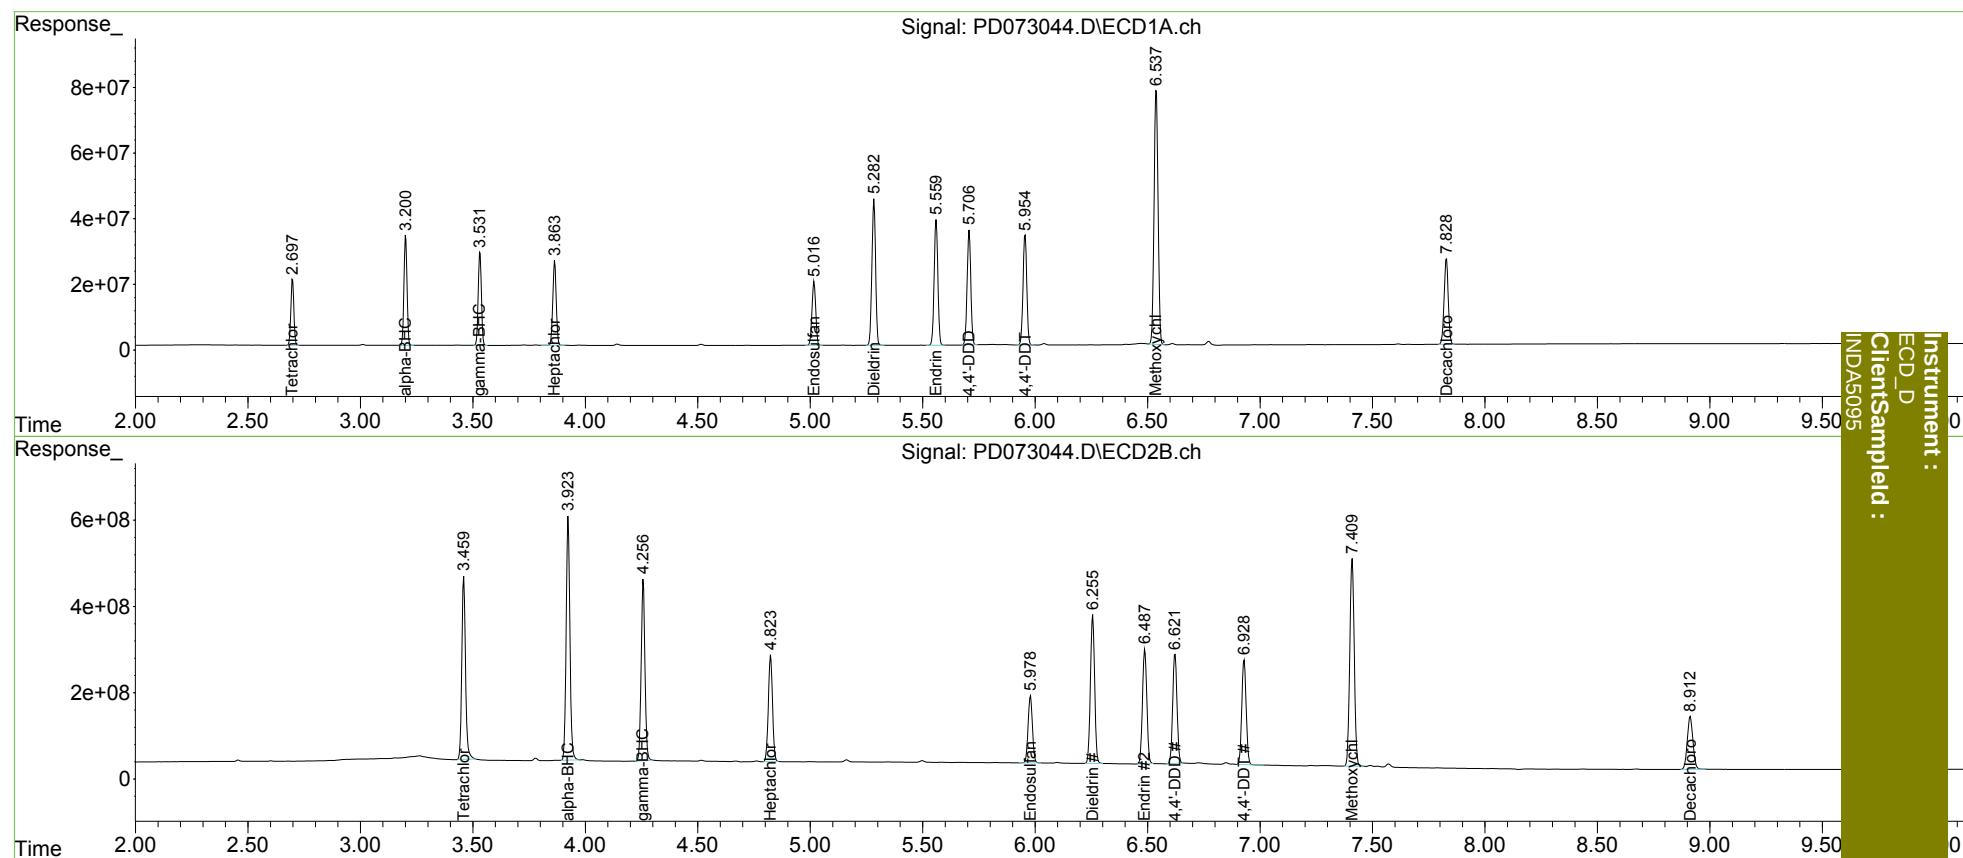

Instrument :
ECD_D
ClientSampled :
INDA5095