

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
 Data File : PD073042.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2022 04:34
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4093

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 06:13:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:13:14 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.699	3.460	91969677	2397.9E6	38.090	36.098
27)	SA Decachlor...	7.829	8.912	169.8E6	1098.6E6	72.790	72.376
Target Compounds							
2)	A alpha-BHC	3.202	3.924	148.7E6	3182.5E6	41.459	35.924
3)	MA gamma-BHC...	3.532	4.257	133.5E6	2456.9E6	40.815	35.385
4)	MA Heptachlor	3.864	4.824	131.9E6	1649.5E6	39.681	34.751
9)	A Endosulfan I	5.017	5.979	109.1E6	1068.9E6	38.483	35.764
13)	MA Dieldrin	5.283	6.256	245.7E6	2253.4E6	80.859	73.408
14)	MA Endrin	5.560	6.488	214.2E6	1822.7E6	79.212	72.215
16)	A 4,4'-DDD	5.707	6.622	192.7E6	1719.3E6	80.546	73.557
17)	MA 4,4'-DDT	5.956	6.930	185.7E6	1640.3E6	84.964	75.511
20)	A Methoxychlor	6.540	7.410	489.5E6	3495.8E6	386.861	364.688

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111722\
Data File : PD073042.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2022 04:34
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 36 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 06:13:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:13:14 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

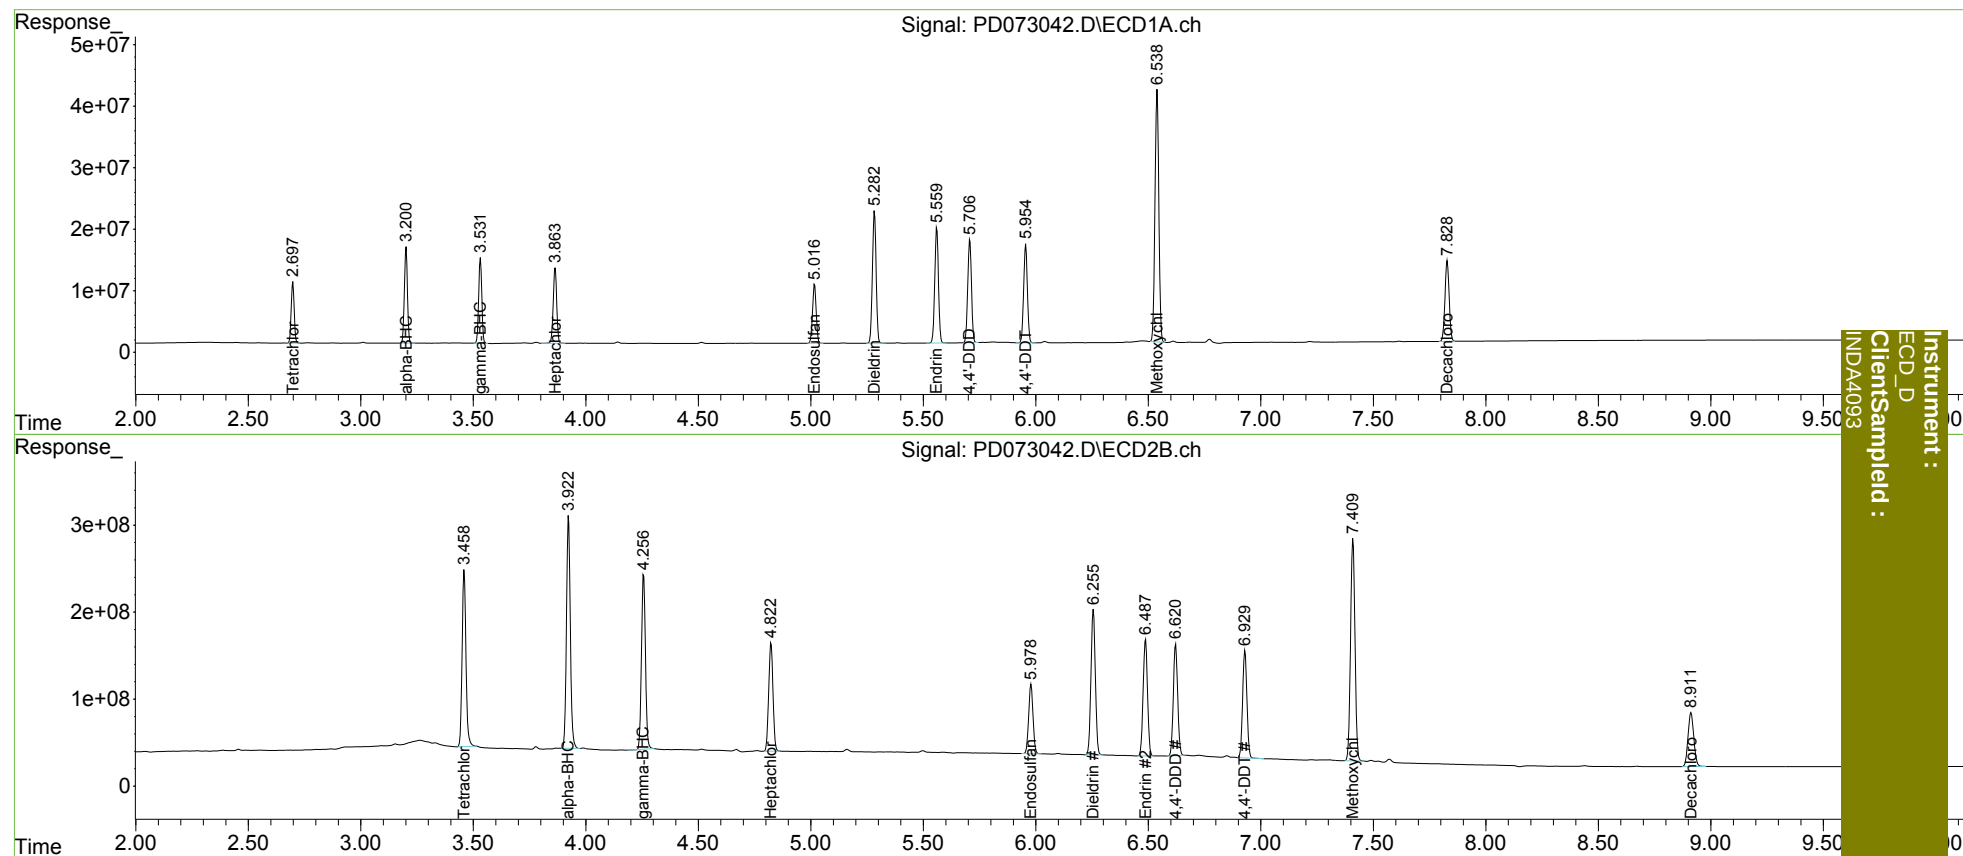

Instrument :
ECD_D
ClientSampled :
INDA4093