

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111723\
 Data File : PD079674.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2023 00:12
 Operator : AR\AJ
 Sample : 05390-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 04:07:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.804	28053088	43435850	19.209	18.990
27)	SA Decachlor...	9.117	7.949	42617134	57050261	24.016	23.896
Target Compounds							
7)	B delta-BHC	0.000	4.183	0	218887	N.D.	<MDL
15)	B Endosulfa...	0.000	5.926f	0	101466	N.D.	<MDL

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111723\
Data File : PD079674.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2023 00:12
Operator : AR\AJ
Sample : 05390-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 04:07:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

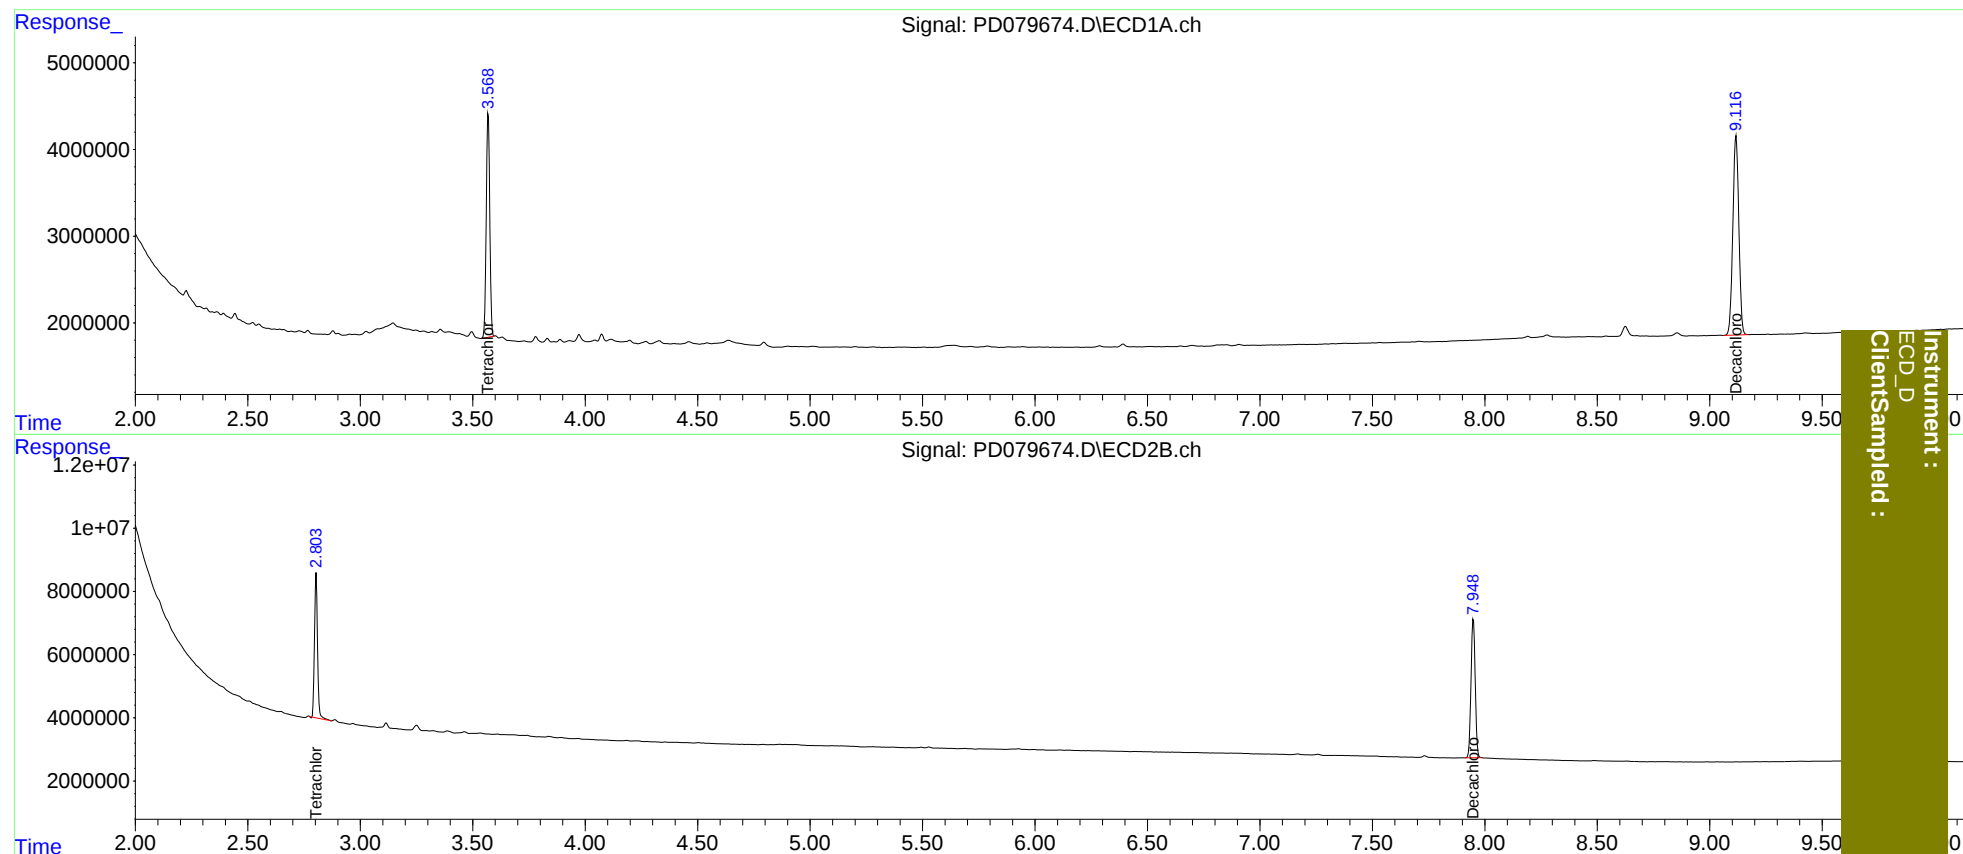


Instrument :
ECD_D
ClientSampled :
0

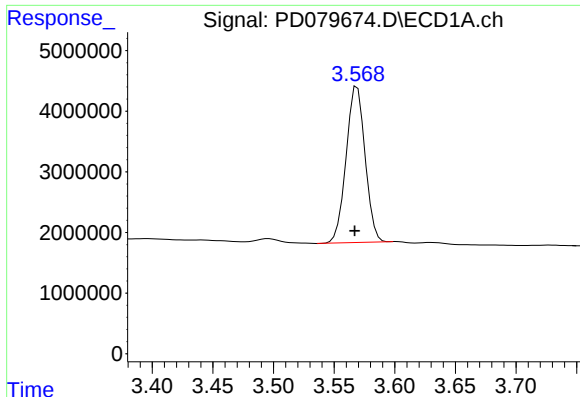

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.002 min
Response: 28053088
Conc: 19.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

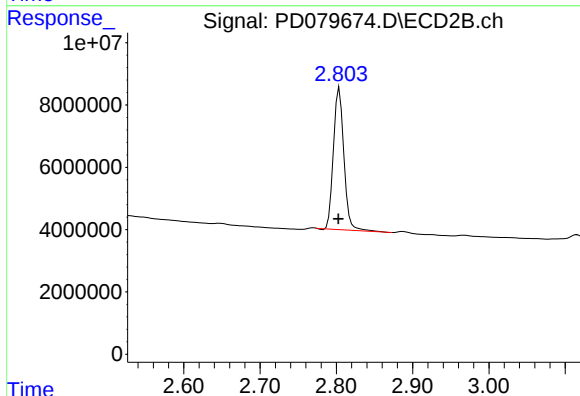


#1 Tetrachloro-m-xylene

R.T.: 2.804 min
Delta R.T.: 0.001 min
Response: 43435850
Conc: 18.99 ng/ml

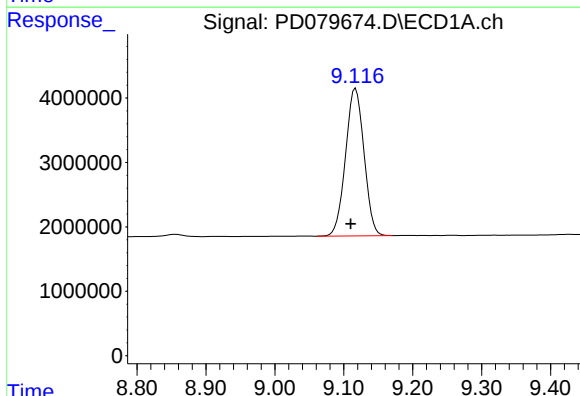

#27 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: 0.007 min
Response: 42617134
Conc: 24.02 ng/ml

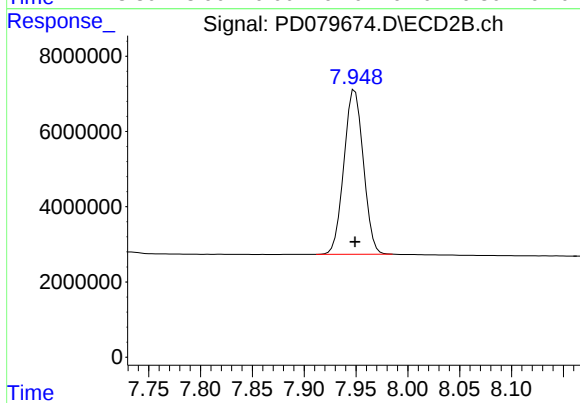

#27 Decachlorobiphenyl

R.T.: 7.949 min
Delta R.T.: 0.000 min
Response: 57050261
Conc: 23.90 ng/ml