

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111723\
 Data File : PD079699.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2023 06:25
 Operator : AR\AJ
 Sample : 05364-17
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 21:52:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.804	28040838	43539907	19.201	19.035
27)	SA Decachlor...	9.117	7.949	40217864	54222338	22.664	22.711
Target Compounds							
2)	A alpha-BHC	0.000	3.324	0	310902	N.D.	<MDL
3)	MA gamma-BHC...	0.000	3.646	0	130586	N.D.	<MDL
4)	MA Heptachlor	0.000	3.968	0	226994	N.D.	<MDL
5)	MB Aldrin	0.000	4.233f	0	579623	N.D.	0.178
6)	B beta-BHC	0.000	3.968f	0	226994	N.D.	0.139
13)	MA Dieldrin	0.000	5.367	0	159160	N.D.	<MDL
14)	MA Endrin	0.000	5.687	0	276511	N.D.	0.101
15)	B Endosulfa...	0.000	5.996	0	870324	N.D.	0.335
19)	B Endosulfa...	0.000	6.353	0	1192294	N.D.	0.480
23)	Toxaphene-2	0.000	5.367	0	159160	N.D.	9.471


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111723\
Data File : PD079699.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2023 06:25
Operator : AR\AJ
Sample : 05364-17
Misc :
ALS Vial : 44 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 21:52:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

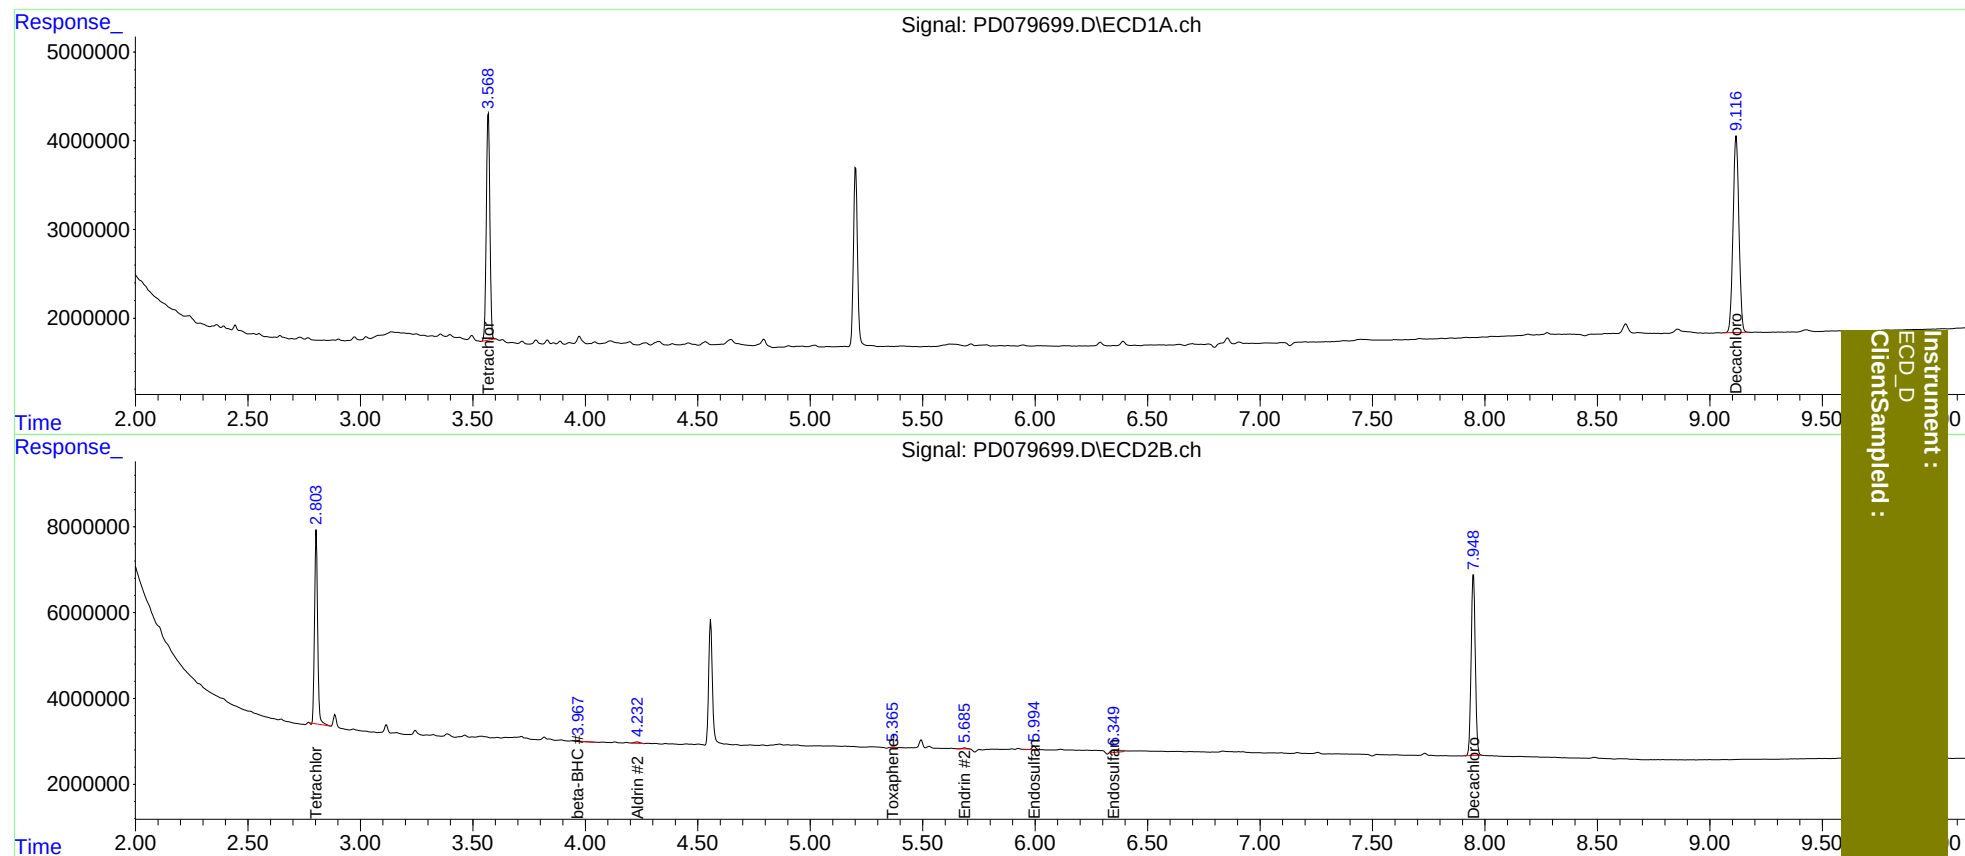


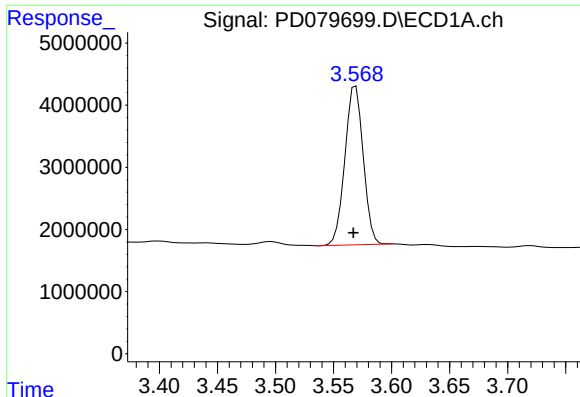

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.002 min
Response: 28040838
Conc: 19.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

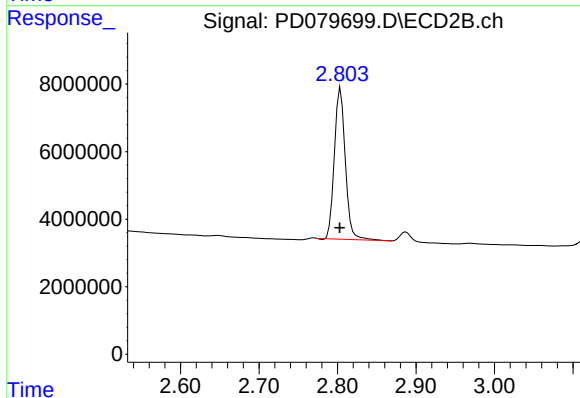


#1 Tetrachloro-m-xylene

R.T.: 2.804 min
Delta R.T.: 0.001 min
Response: 43539907
Conc: 19.04 ng/ml

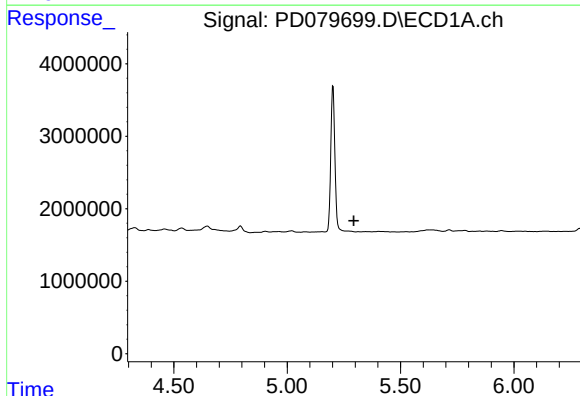


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.294 min
Response: 0
Conc: N.D.

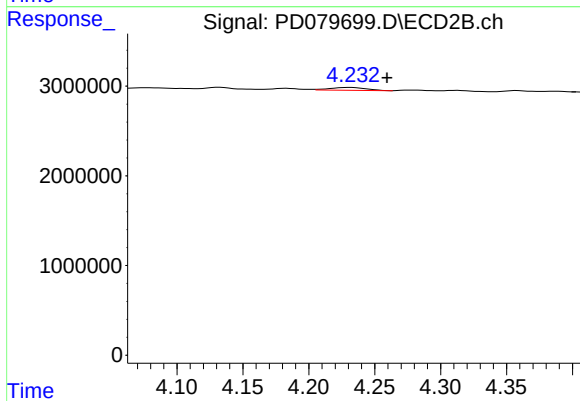

#5 Aldrin


R.T.: 4.233 min
Delta R.T.: -0.027 min
Response: 579623
Conc: 0.18 ng/ml

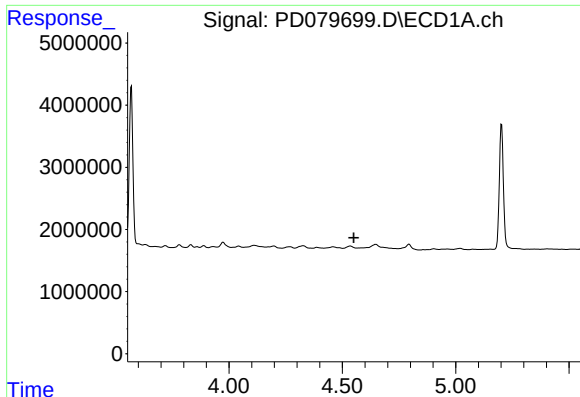

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.551 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

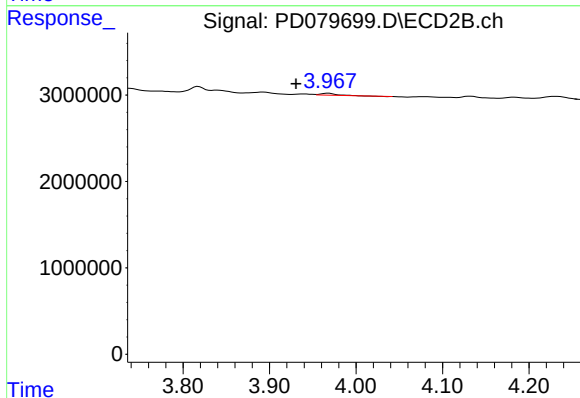


#6 beta-BHC

R.T.: 3.968 min
Delta R.T.: 0.037 min
Response: 226994
Conc: 0.14 ng/ml

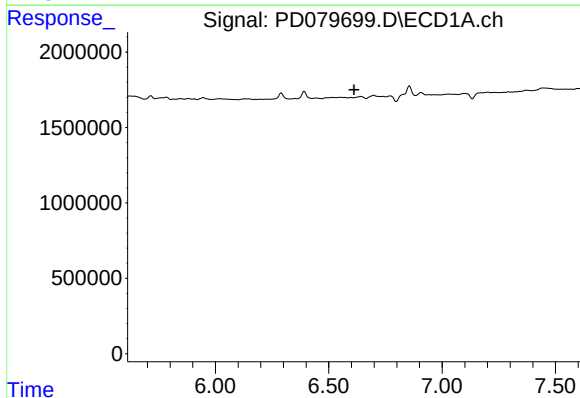


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.612 min
Response: 0
Conc: N.D.

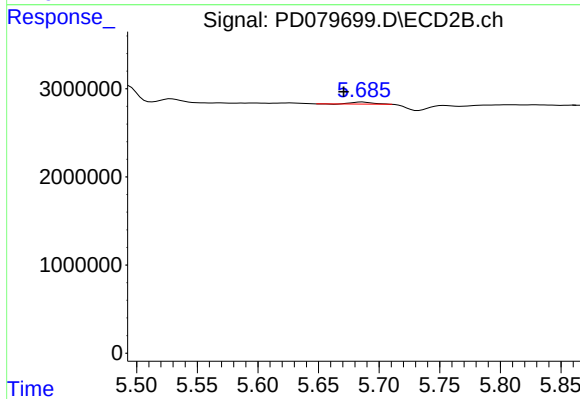

#14 Endrin


R.T.: 5.687 min
Delta R.T.: 0.016 min
Response: 276511
Conc: 0.10 ng/ml

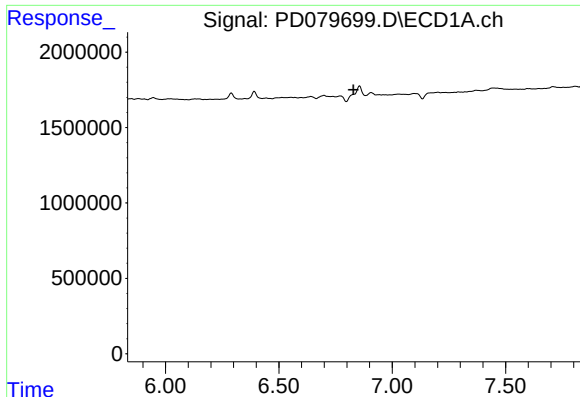

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.830 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

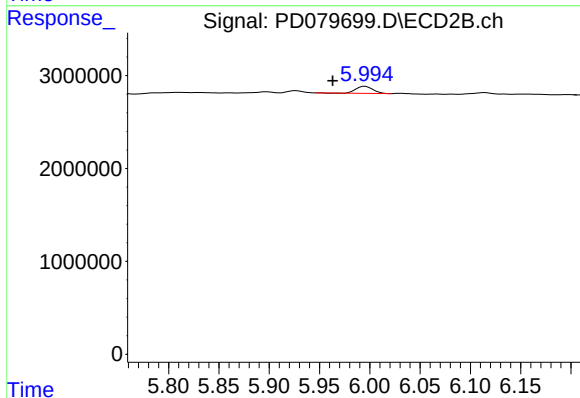


#15 Endosulfan II

R.T.: 5.996 min
Delta R.T.: 0.032 min
Response: 870324
Conc: 0.34 ng/ml

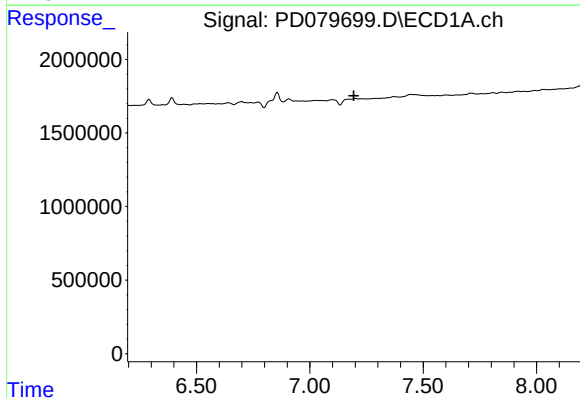


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 7.193 min
Response: 0
Conc: N.D.

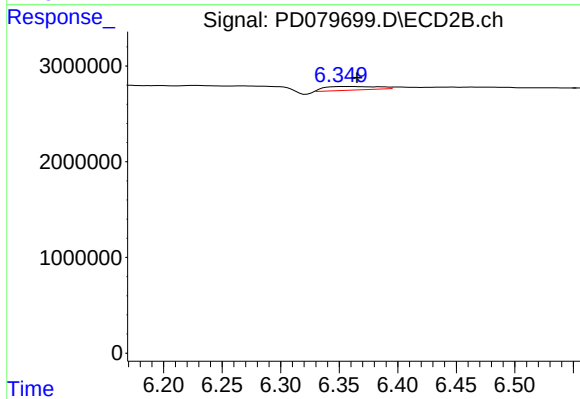

#19 Endosulfan Sulfate


R.T.: 6.353 min
Delta R.T.: -0.012 min
Response: 1192294
Conc: 0.48 ng/ml

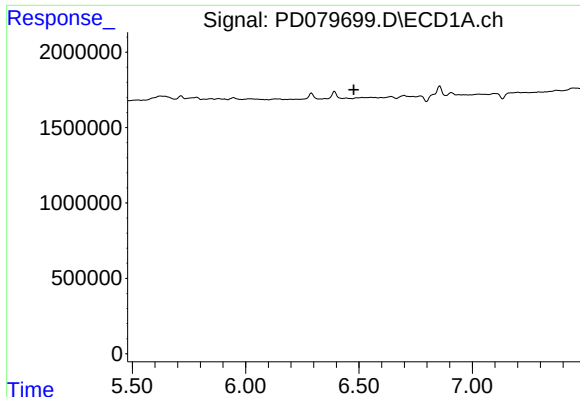

#23 Toxaphene-2


R.T.: 0.000 min
Exp R.T.: 6.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

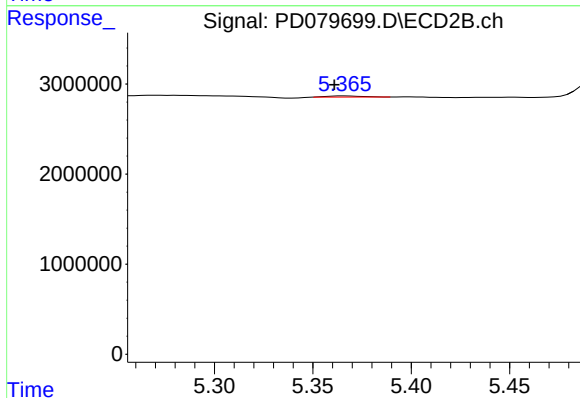


#23 Toxaphene-2

R.T.: 5.367 min
Delta R.T.: 0.006 min
Response: 159160
Conc: 9.47 ng/ml

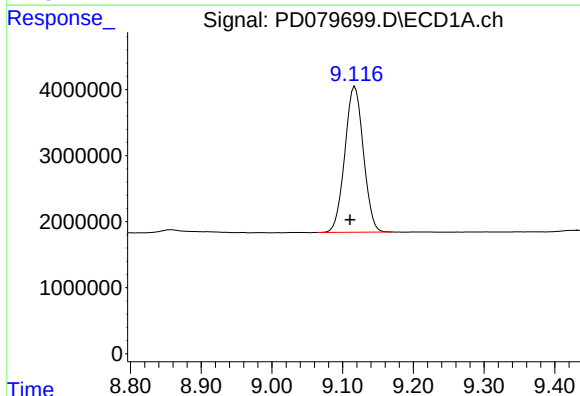

#27 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: 0.007 min
Response: 40217864
Conc: 22.66 ng/ml

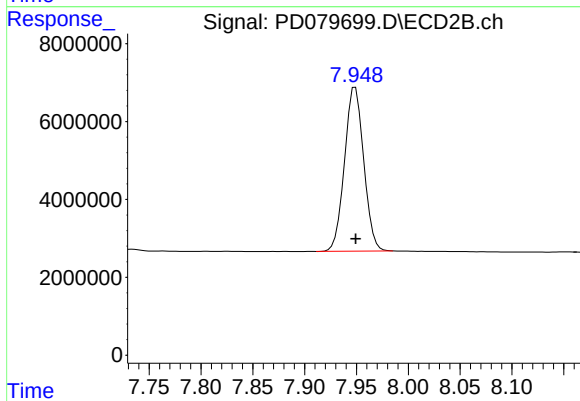

#27 Decachlorobiphenyl

R.T.: 7.949 min
Delta R.T.: 0.000 min
Response: 54222338
Conc: 22.71 ng/ml