

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111723\
Data File : PD079686.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2023 03:05
Operator : AR\AJ
Sample : 05364-07
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
C0QH5

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 11/20/2023
Supervised By :Ankita Jodhani 11/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 04:11:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

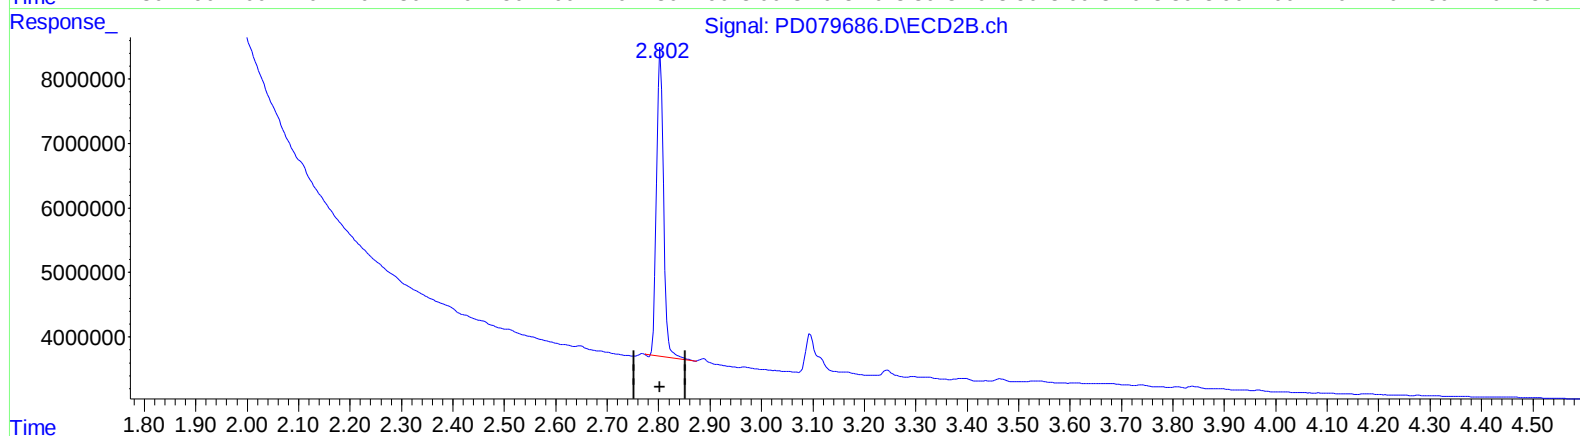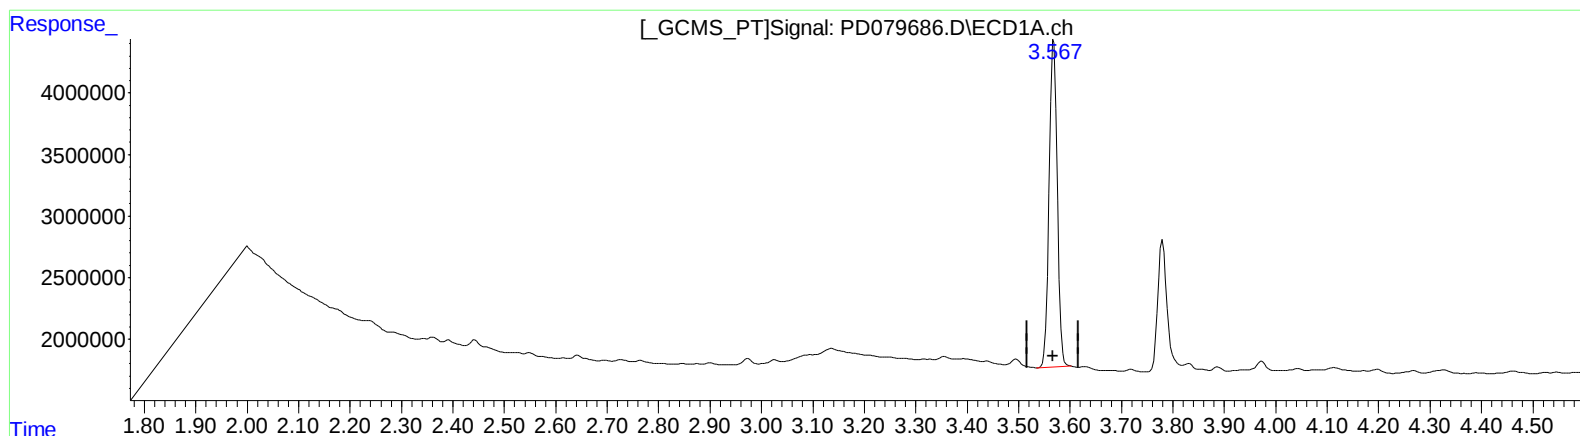

QEdit

(1) Tetrachloro-m-xylene (SA)

3.569min 20.096 ng/ml

response 29347956

(1) Tetrachloro-m-xylene #2 (SA)

2.804min 20.027 ng/ml

response 45807742

(+) = Expected Retention Time

PD110623CLP.M Sat Nov 18 04:52:11 2023

Page: 1

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111723\
Data File : PD079686.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2023 03:05
Operator : AR\AJ
Sample : 05364-07
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
C0QH5

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 11/20/2023
Supervised By :Ankita Jodhani 11/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 04:11:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

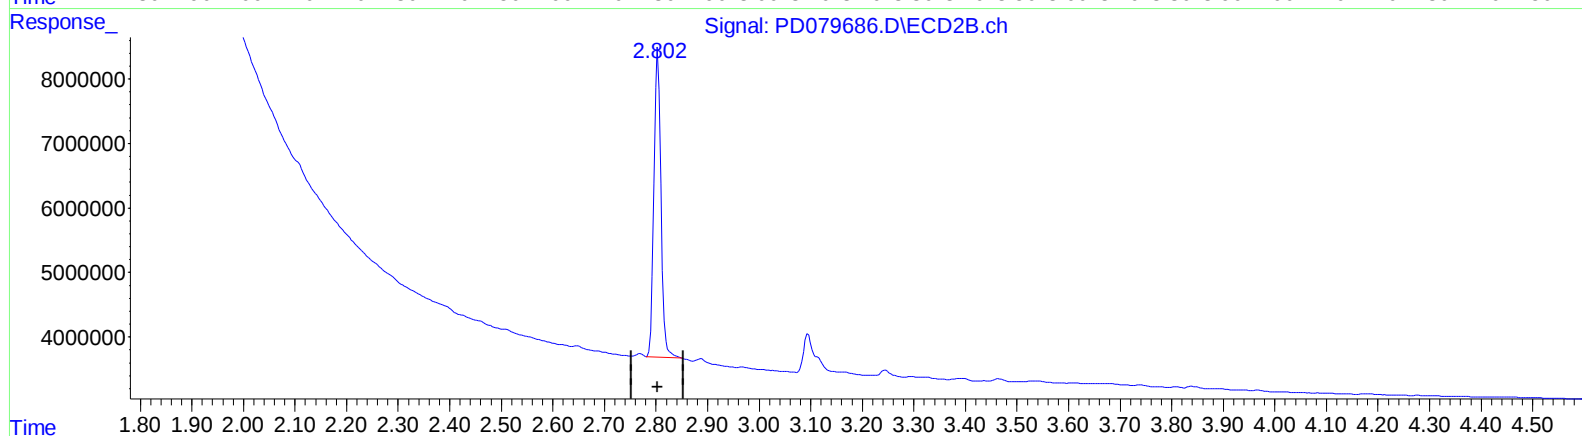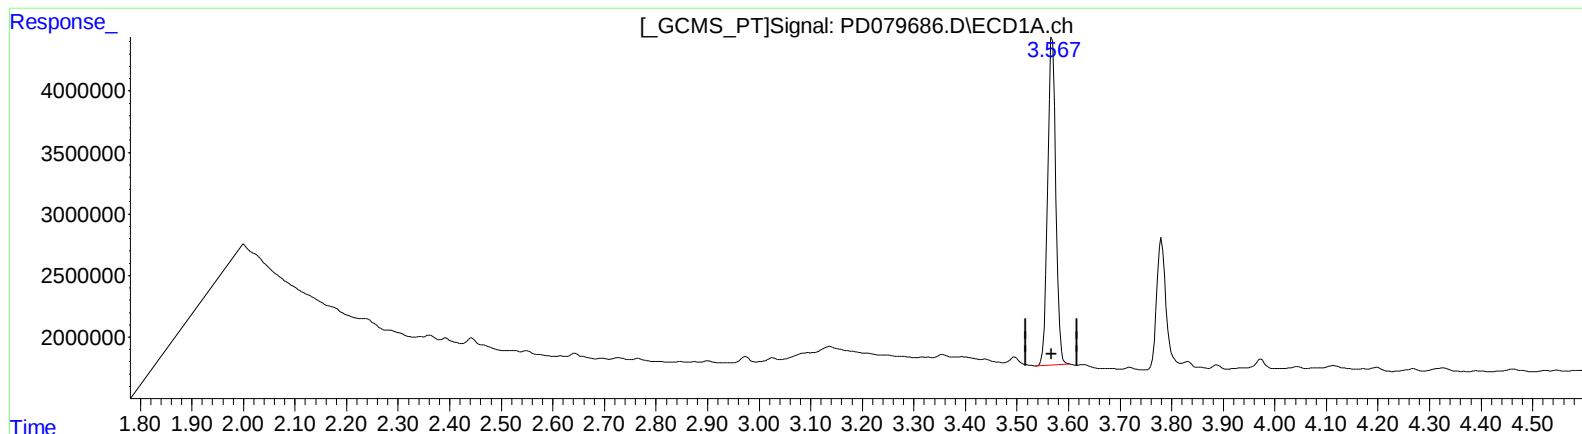

QEdit

(1) Tetrachloro-m-xylene (SA)

3.569min 20.096 ng/ml

response 29347956

(1) Tetrachloro-m-xylene #2 (SA)

2.802min 20.021 ng/ml m

response 45794411

(+) = Expected Retention Time

PD110623CLP.M Sat Nov 18 04:52:31 2023

Page: 1