

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111723\
 Data File : PD079665.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2023 22:12
 Operator : AR\AJ
 Sample : 05328-14MS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A49W2MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 00:28:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.804	21735563	33884192	14.884	14.814
2)	SA Decachlor...	9.117	7.949	31888948	43687737	17.970	18.299
Target Compounds							
2)	A alpha-BHC	4.026	3.307	100.5E6	152.9E6	40.579	42.175
3)	MA gamma-BHC...	4.360	3.637	92728024	138.7E6	39.248	40.376
4)	MA Heptachlor	4.952	3.979	91153760	128.5E6	36.394	38.517
5)	MB Aldrin	5.296	4.260	86838364	124.3E6	37.031	38.192
6)	B beta-BHC	4.552	3.931	39139404	57220049	36.046	34.940
7)	B delta-BHC	4.802	4.163	95461142	141.0E6	38.308	39.471
8)	B Heptachlo...	5.722	4.761	85111162	123.8E6	38.392	40.013
9)	A Endosulfan I	6.109	5.132	80991615	111.6E6	39.179	40.264
10)	B trans-Chl...	5.977	5.012	82006638	120.0E6	38.542	40.413
11)	B cis-Chlor...	6.058	5.076	83809258	118.8E6	38.481	39.132
12)	B 4,4'-DDE	6.228	5.265	159.2E6	238.3E6	80.621	85.105
13)	MA Dieldrin	6.384	5.397	175.5E6	261.4E6	79.767	82.091
14)	MA Endrin	6.615	5.672	144.9E6	230.9E6	79.418	84.311
15)	B Endosulfa...	6.832	5.964	149.7E6	222.0E6	78.690	85.483
16)	A 4,4'-DDD	6.745	5.818	131.1E6	201.4E6	80.948	85.541
17)	MA 4,4'-DDT	7.060	6.070	136.9E6	199.3E6	80.351	82.989
18)	B Endrin al...	6.962	6.143	109.8E6	160.6E6	73.661	79.358
19)	B Endosulfa...	7.197	6.365	143.0E6	206.1E6	76.807	82.955
20)	A Methoxychlor	7.535	6.645	344.1E6	489.9E6	373.226	381.121
21)	B Endrin ke...	7.683	6.872	153.9E6	239.9E6	78.777	84.370

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111723\
Data File : PD079665.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2023 22:12
Operator : AR\AJ
Sample : 05328-14MS
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 00:28:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

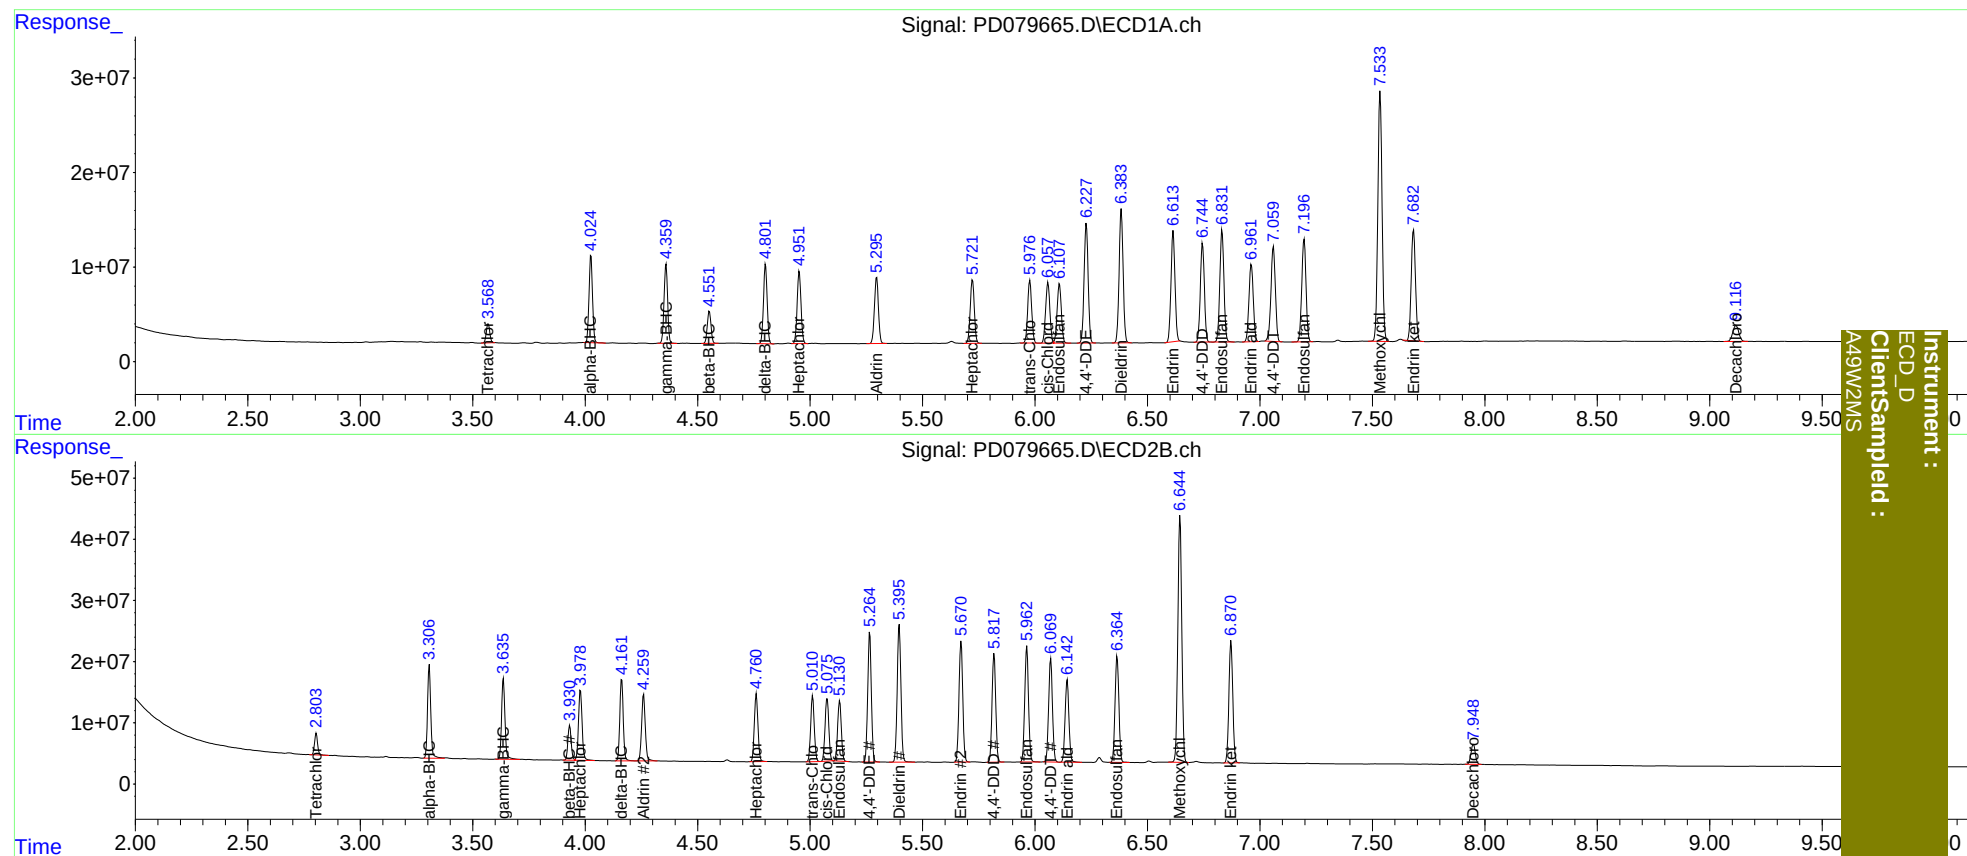

Instrument :
ECD_D
ClientSampled :
A49W2MS