

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111723\
 Data File : PD079672.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2023 23:45
 Operator : AR\AJ
 Sample : 05390-05MS
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0TJ7MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 00:31:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.804	26883732	41826657	18.409	18.286
27)	SA Decachlor...	9.117	7.949	41076616	55380586	23.148	23.196
Target Compounds							
2)	A alpha-BHC	4.025	3.307	120.2E6	181.7E6	48.522	50.108
3)	MA gamma-BHC...	4.359	3.636	110.4E6	164.2E6	46.748	47.791
4)	MA Heptachlor	4.952	3.978	111.7E6	158.2E6	44.609	47.415
5)	MB Aldrin	5.296	4.259	107.9E6	155.5E6	46.006	47.801
6)	B beta-BHC	4.552	3.931	46765964	69391304	43.070	42.372
7)	B delta-BHC	4.802	4.162	113.4E6	167.9E6	45.515	46.981
8)	B Heptachlo...	5.722	4.761	101.4E6	148.2E6	45.718	47.914
9)	A Endosulfan I	6.108	5.131	96222391	132.7E6	46.547	47.874
10)	B trans-Chl...	5.978	5.011	98299022	143.9E6	46.199	48.456
11)	B cis-Chlor...	6.058	5.076	100.3E6	142.6E6	46.073	46.981
12)	B 4,4'-DDE	6.229	5.264	191.5E6	285.9E6	96.976	102.104
13)	MA Dieldrin	6.384	5.396	208.7E6	308.9E6	94.860	97.002
14)	MA Endrin	6.615	5.671	167.1E6	263.9E6	91.563	96.357
15)	B Endosulfa...	6.832	5.963	177.0E6	263.5E6	93.037	101.441
16)	A 4,4'-DDD	6.746	5.818	157.1E6	239.9E6	96.962	101.922
17)	MA 4,4'-DDT	7.061	6.070	163.0E6	236.2E6	95.678	98.328
18)	B Endrin al...	6.963	6.143	130.9E6	192.7E6	87.803	95.217
19)	B Endosulfa...	7.197	6.365	169.7E6	242.2E6	91.144	97.467
20)	A Methoxychlor	7.535	6.645	398.9E6	561.4E6	432.707	436.759
21)	B Endrin ke...	7.684	6.872	182.3E6	285.9E6	93.306	100.570

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111723\
Data File : PD079672.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2023 23:45
Operator : AR\AJ
Sample : 05390-05MS
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 00:31:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

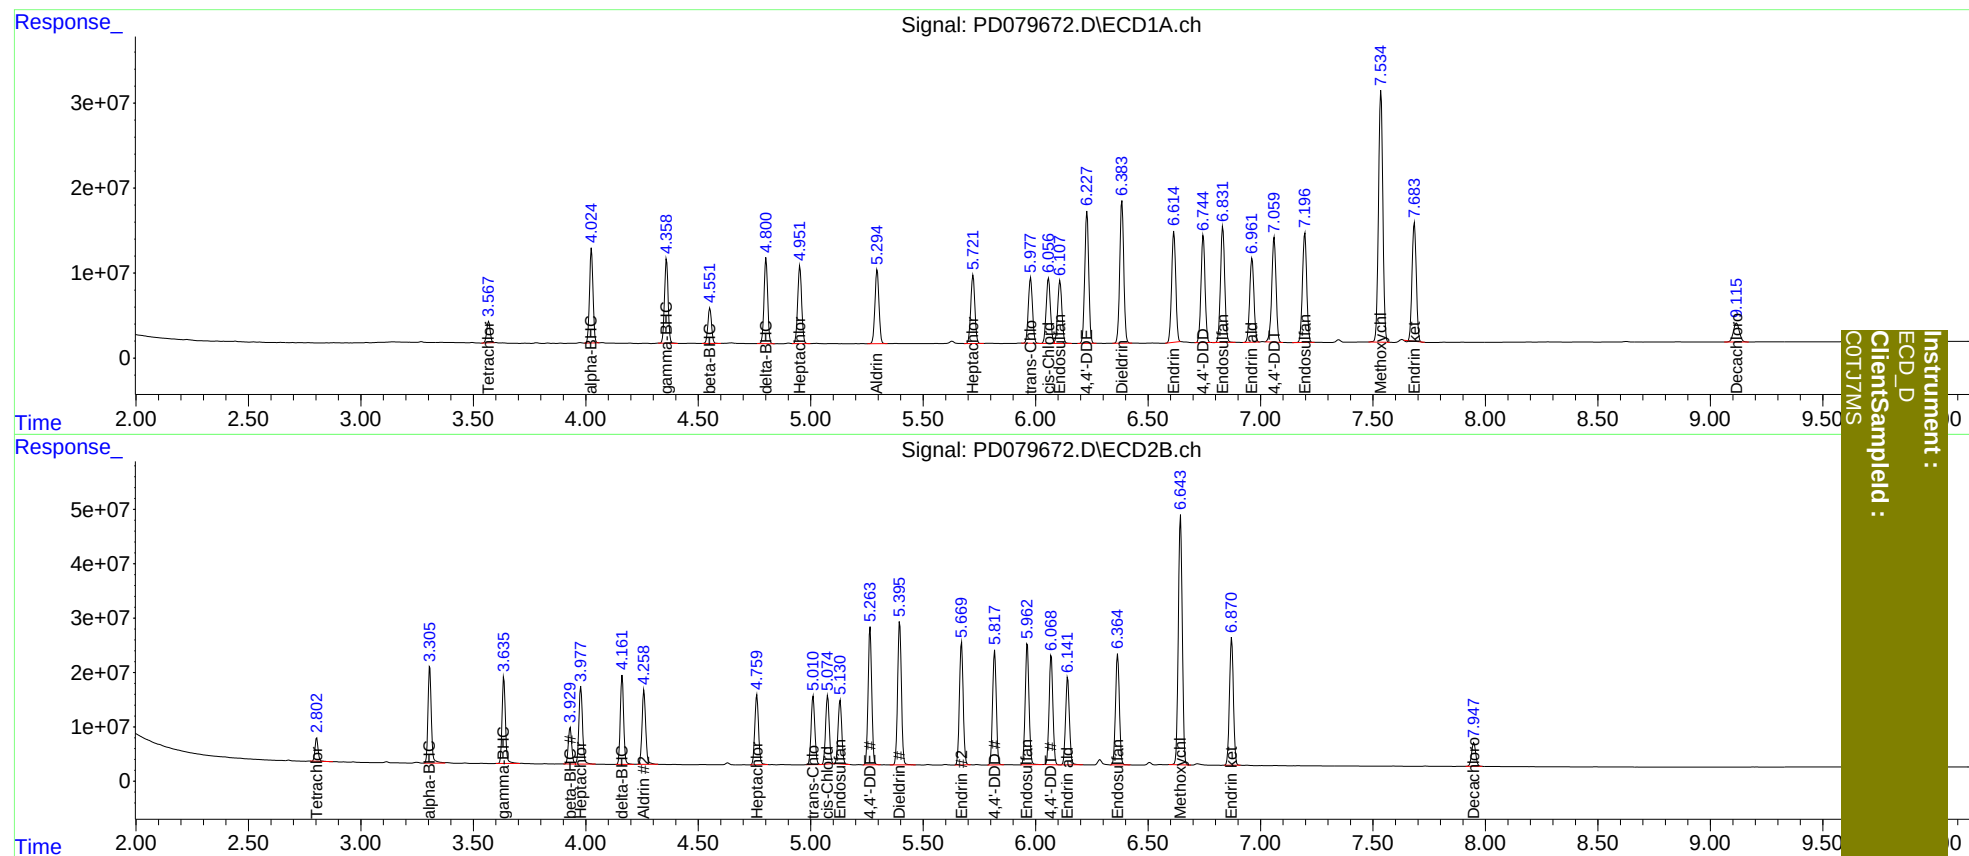

Instrument :
ECD_D
ClientSampled :
COTJMS