

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111723\
 Data File : PD079673.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2023 23:59
 Operator : AR\AJ
 Sample : 05390-06MSD
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0TJ7MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 04:07:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.804	26814992	41699487	18.362	18.231
2)	SA Decachlor...	9.117	7.949	41172678	55431730	23.202	23.218
Target Compounds							
2)	A alpha-BHC	4.026	3.307	120.1E6	180.3E6	48.461	49.718
3)	MA gamma-BHC...	4.359	3.636	110.3E6	163.3E6	46.673	47.540
4)	MA Heptachlor	4.952	3.978	111.4E6	157.8E6	44.476	47.292
5)	MB Aldrin	5.295	4.259	107.7E6	155.4E6	45.911	47.771
6)	B beta-BHC	4.552	3.931	46730841	69048441	43.038	42.163
7)	B delta-BHC	4.802	4.162	112.9E6	167.2E6	45.293	46.802
8)	B Heptachlo...	5.721	4.761	101.2E6	147.5E6	45.627	47.673
9)	A Endosulfan I	6.109	5.131	95975582	132.0E6	46.428	47.613
10)	B trans-Chl...	5.978	5.011	98007903	143.5E6	46.062	48.349
11)	B cis-Chlor...	6.058	5.076	100.0E6	141.9E6	45.919	46.747
12)	B 4,4'-DDE	6.228	5.265	190.6E6	284.6E6	96.525	101.650
13)	MA Dieldrin	6.384	5.396	207.8E6	308.3E6	94.470	96.811
14)	MA Endrin	6.614	5.671	167.1E6	263.6E6	91.567	96.248
15)	B Endosulfa...	6.832	5.964	176.4E6	262.9E6	92.731	101.240
16)	A 4,4'-DDD	6.746	5.818	156.4E6	238.6E6	96.548	101.369
17)	MA 4,4'-DDT	7.060	6.070	163.1E6	236.2E6	95.730	98.318
18)	B Endrin al...	6.962	6.143	130.4E6	192.1E6	87.462	94.910
19)	B Endosulfa...	7.196	6.365	169.2E6	241.6E6	90.850	97.238
20)	A Methoxychlor	7.535	6.645	399.7E6	563.3E6	433.542	438.267
21)	B Endrin ke...	7.684	6.872	182.6E6	285.5E6	93.474	100.410

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111723\
Data File : PD079673.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2023 23:59
Operator : AR\AJ
Sample : 05390-06MSD
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 04:07:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

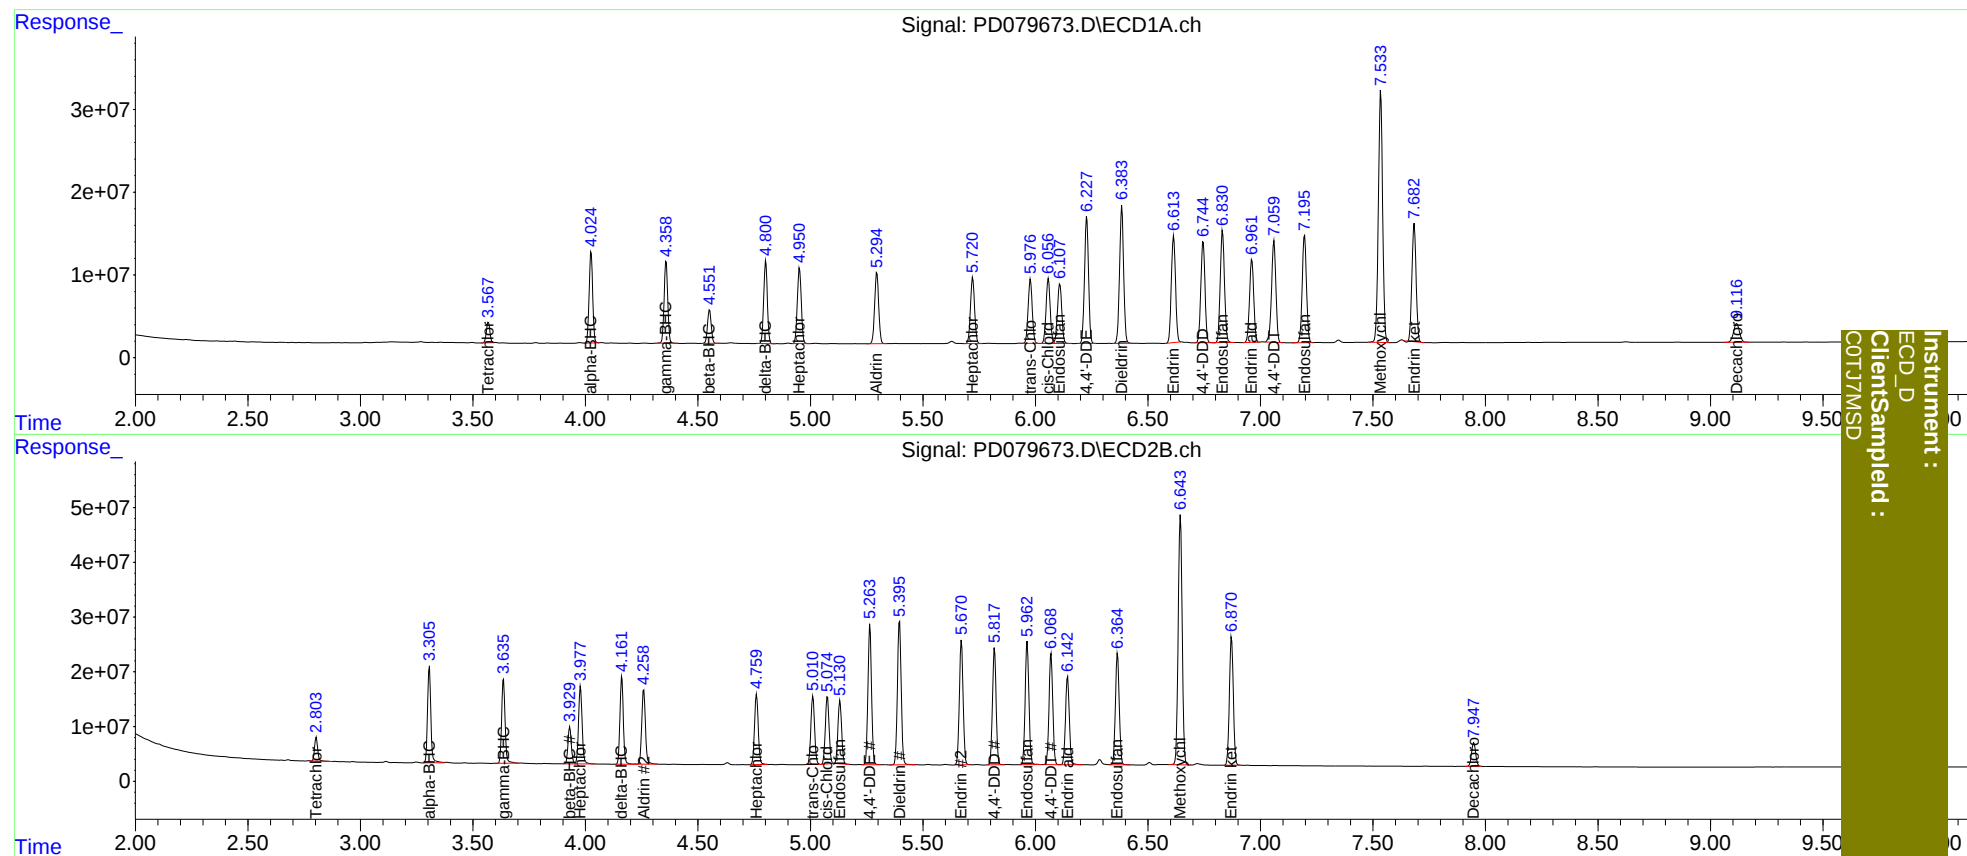

Instrument :
ECD_D
ClientSampled :
COTJMSD