

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111723\
 Data File : PD079682.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2023 02:12
 Operator : AR\AJ
 Sample : 05364-03MSD
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0QJ6MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/20/2023
 Supervised By : Ankita Jodhani 11/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 04:10:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.804	28268530	50152473	19.357	21.926
27)	SA Decachlor...	9.118	7.949	43453954	58482553	24.487	24.496
Target Compounds							
2)	A alpha-BHC	4.026	3.307	133.3E6	200.3E6	53.787	55.252
3)	MA gamma-BHC...	4.359	3.636	120.2E6	181.3E6	50.876	52.759
4)	MA Heptachlor	4.953	3.979	119.6E6	170.1E6	47.759	50.998
5)	MB Aldrin	5.296	4.260	115.2E6	166.4E6	49.140	51.126
6)	B beta-BHC	4.553	3.931	50573495	75841304	46.577	46.311
7)	B delta-BHC	4.803	4.162	124.8E6	184.9E6	50.062	51.751
8)	B Heptachlo...	5.723	4.761	110.8E6	162.1E6	49.984	52.423
9)	A Endosulfan I	6.109	5.132	105.1E6	146.6E6	50.852	52.878
10)	B trans-Chl...	5.978	5.012	106.4E6	156.3E6	49.983	52.641
11)	B cis-Chlor...	6.059	5.076	108.9E6	155.5E6	50.003	51.238
12)	B 4,4'-DDE	6.229	5.265	207.6E6	310.0E6	105.172	110.704
13)	MA Dieldrin	6.384	5.396	228.1E6	340.2E6	103.673	106.854
14)	MA Endrin	6.615	5.671	181.0E6	286.3E6	99.193	104.532
15)	B Endosulfa...	6.833	5.963	193.7E6	289.6E6	101.820	111.495
16)	A 4,4'-DDD	6.746	5.818	170.6E6	263.1E6	105.291	111.743
17)	MA 4,4'-DDT	7.061	6.070	177.0E6	257.4E6	103.922	107.146
18)	B Endrin al...	6.963	6.143	141.7E6	209.5E6	95.064	103.520
19)	B Endosulfa...	7.197	6.365	185.3E6	265.9E6	99.532	107.003
20)	A Methoxychlor	7.536	6.644	430.9E6	605.5E6	467.420	471.044
21)	B Endrin ke...	7.684	6.872	204.2E6	314.5E6	104.490m	110.624

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111723\
Data File : PD079682.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2023 02:12
Operator : AR\AJ
Sample : 05364-03MSD
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 04:10:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

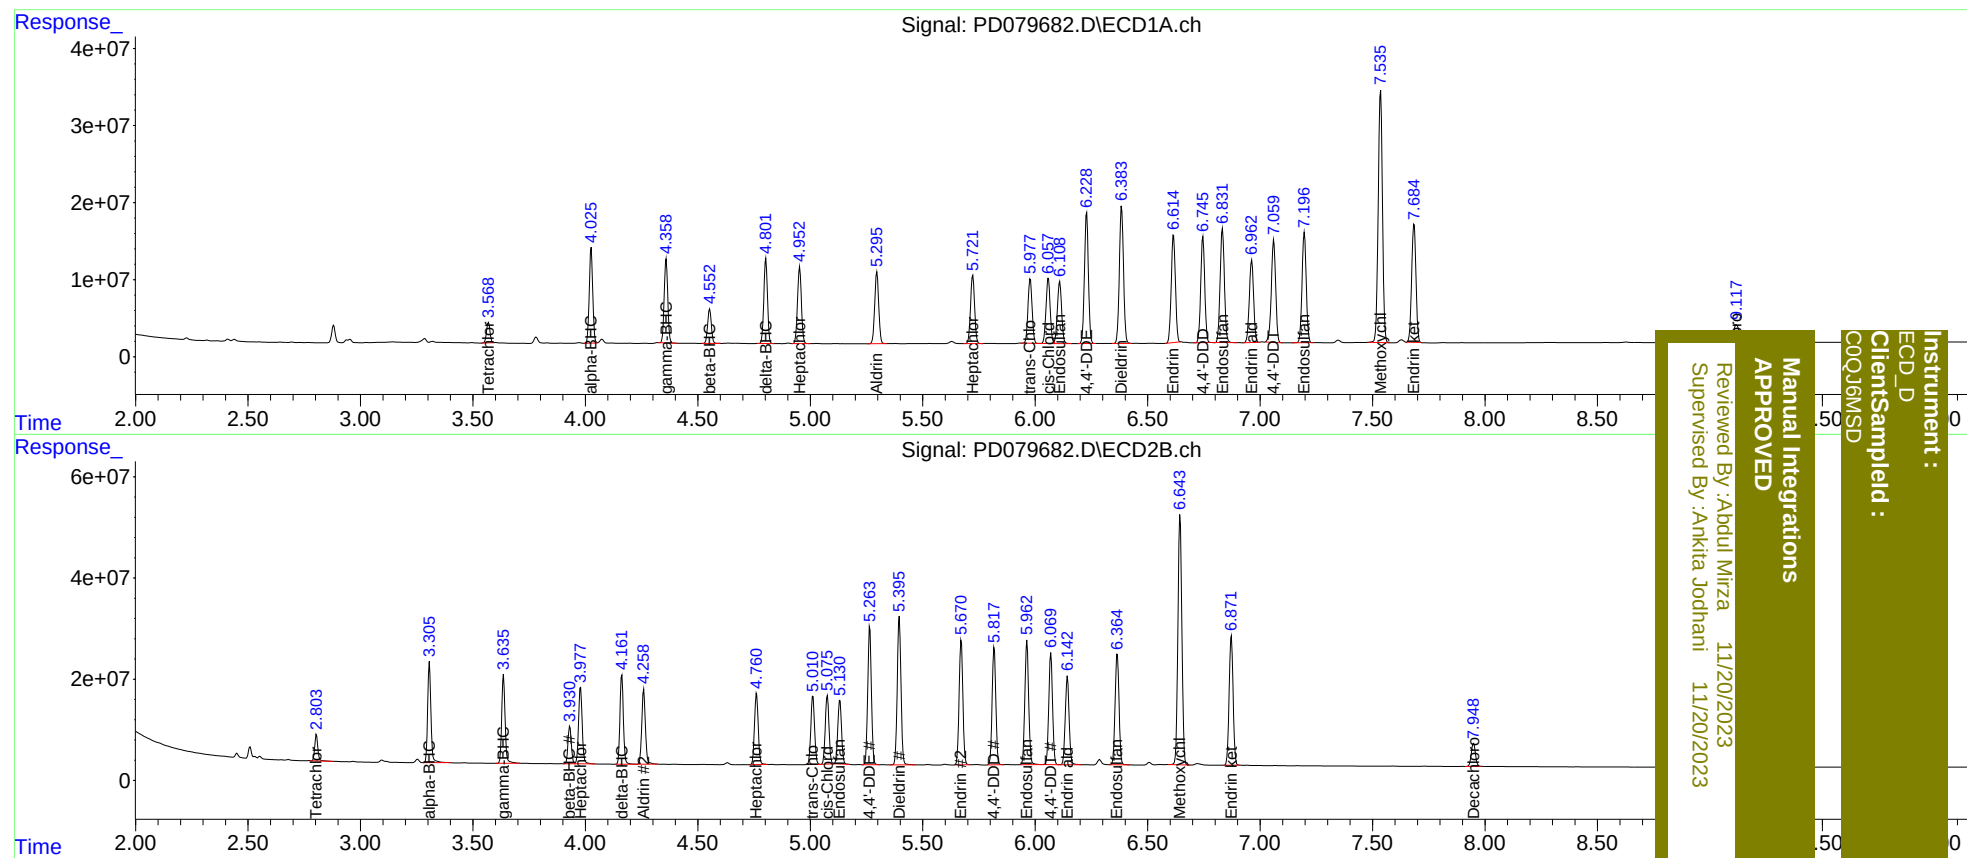

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 11/20/2023
Supervised By: Ankita Jodhani 11/20/2023

Instrument :
ECD_D
ClientSampled :
COQJ6MSD