

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111819\
 Data File : PD056068.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2019 14:39
 Operator : SG\AJ
 Sample : K5820-22
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0B17

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 01:29:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.963	13780461	18004351	18.306	17.181
27)	SA Decachlor...	7.966	9.001	21786095	26966755	26.728	23.747
Target Compounds							
10)	B trans-Chl...	0.000	6.045	0	1781635	N.D.	1.249


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111819\
Data File : PD056068.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2019 14:39
Operator : SG\AJ
Sample : K5820-22
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0B17

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:29:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

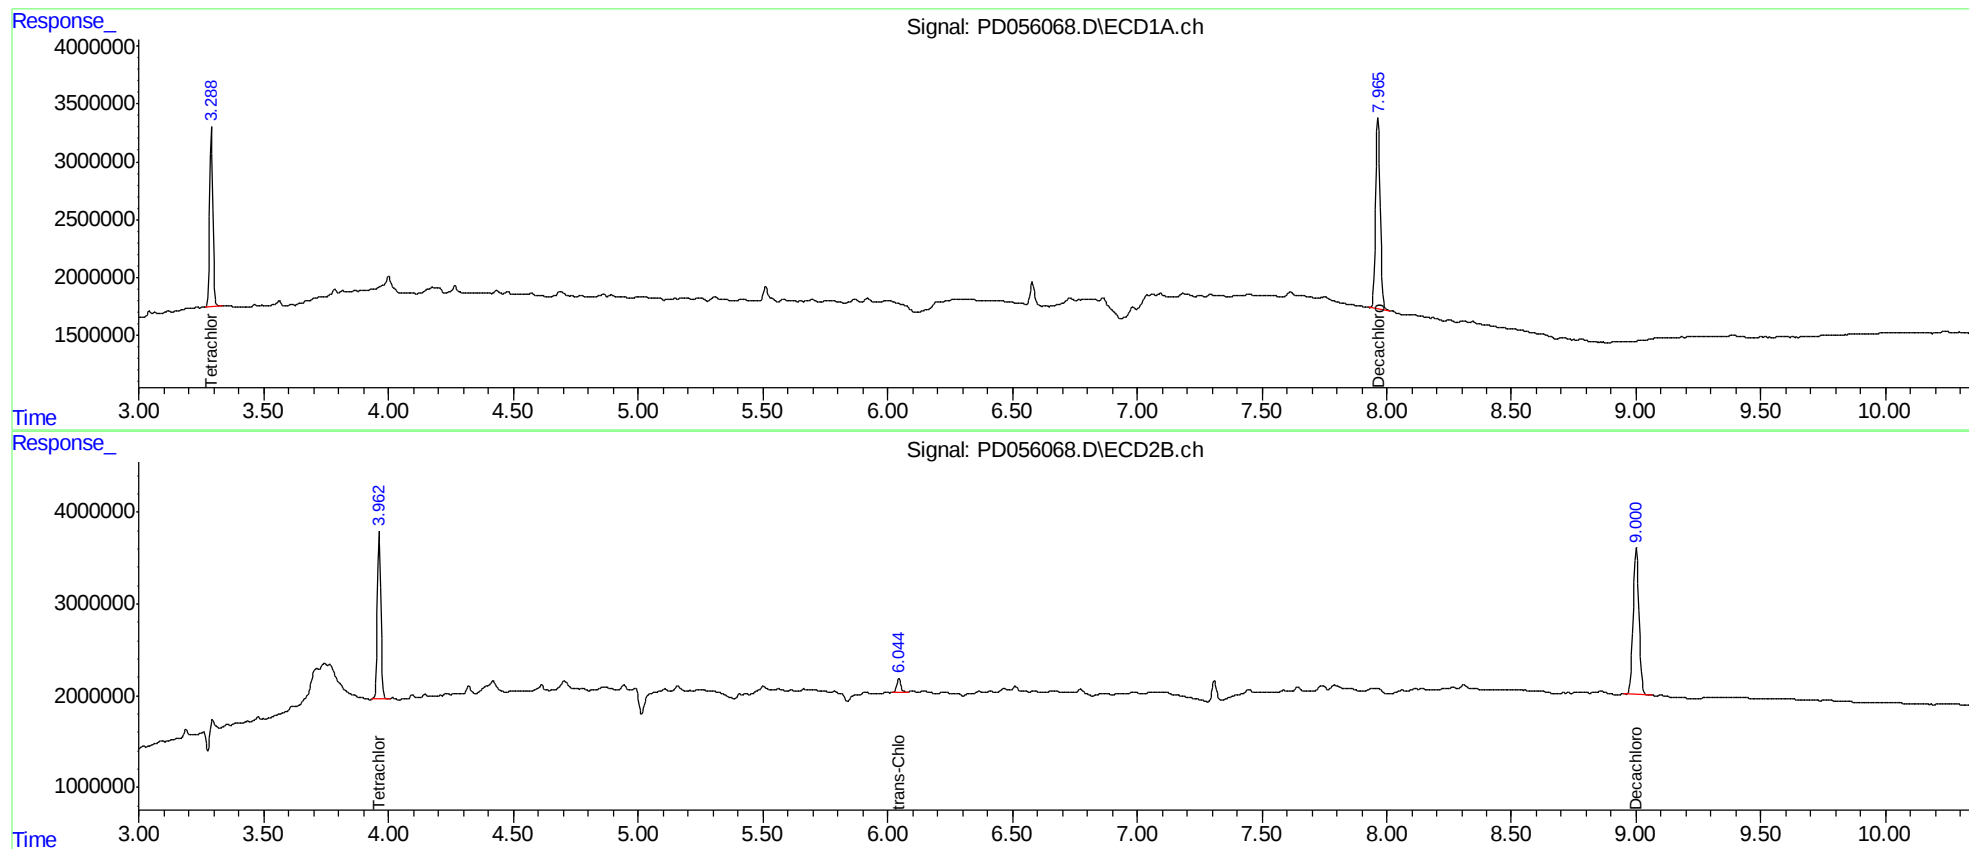


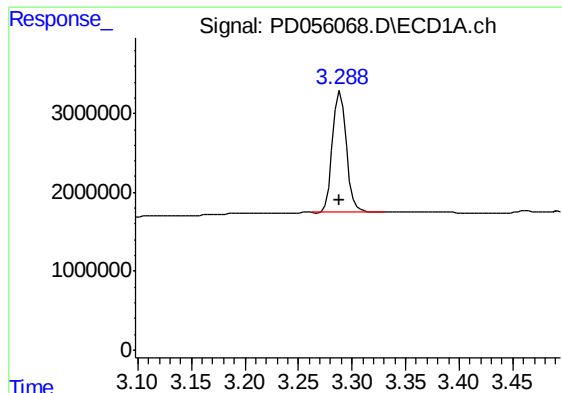

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 13780461
Conc: 18.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0B17

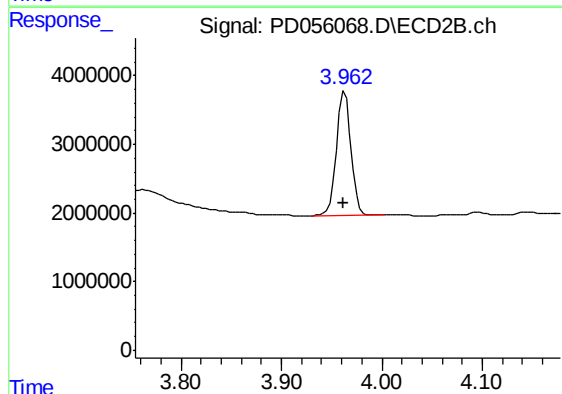


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.002 min
Response: 18004351
Conc: 17.18 ng/ml

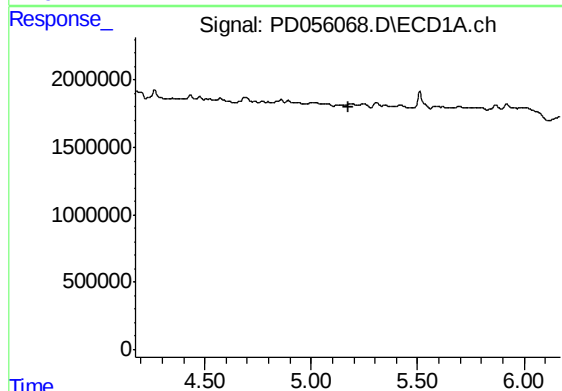


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

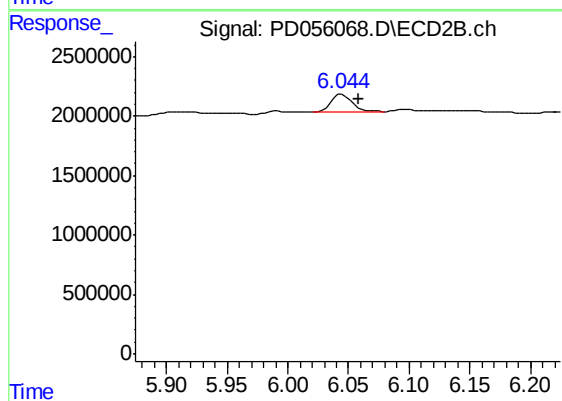

#10 trans-Chlordane


R.T.: 6.045 min
Delta R.T.: -0.013 min
Response: 1781635
Conc: 1.25 ng/ml

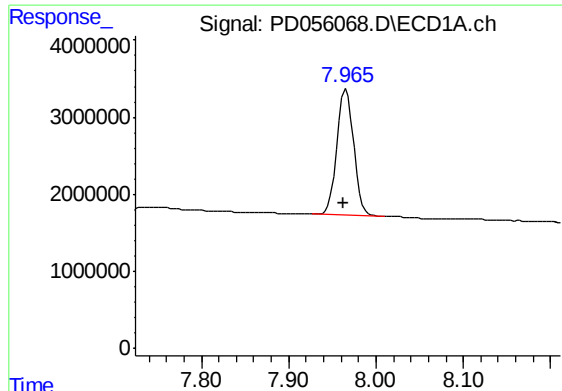

#27 Decachlorobiphenyl

R.T.: 7.966 min
Delta R.T.: 0.003 min
Response: 21786095
Conc: 26.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0B17

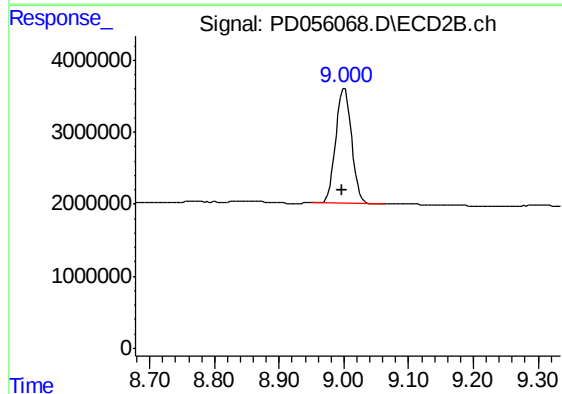

#27 Decachlorobiphenyl

R.T.: 9.001 min
Delta R.T.: 0.004 min
Response: 26966755
Conc: 23.75 ng/ml