

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111819\
 Data File : PD056073.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2019 17:20
 Operator : SG\AJ
 Sample : K5820-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AY8

Manual Integrations
 APPROVED

Ankita
 11/19/2019 1:06:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 01:30:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.287	3.961	16474779	20047646	21.885m	19.130m
27) SA Decachlor...	7.966	8.999	21893800	30140885	26.860	26.543m
Target Compounds						
3) MA gamma-BHC...	3.998	4.612	13451849	10307230	13.151	7.316m#
14) MA Endrin	5.774	6.652	3355689	7567799	4.183m	6.573m#
16) A 4,4'-DDD	5.916	6.771	19492294	29859360	27.599m	26.740m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111819\
Data File : PD056073.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2019 17:20
Operator : SG\AJ
Sample : K5820-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:30:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

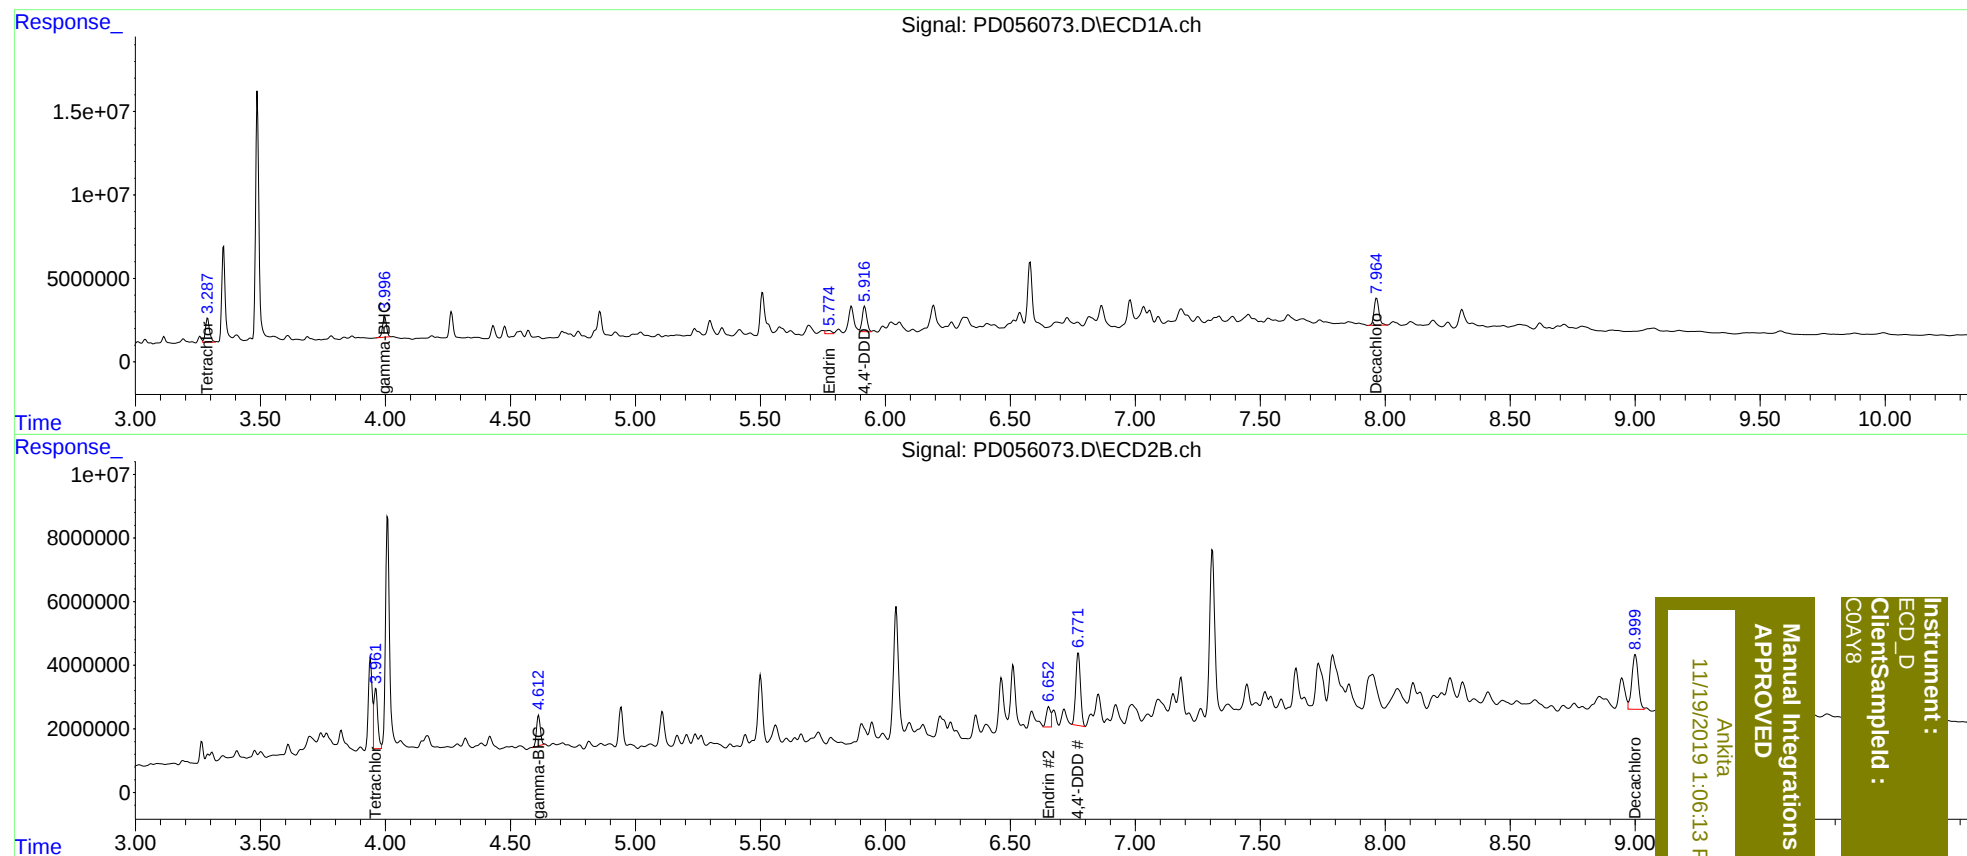

11/19/2019 1:06:13 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client Sampled :
C0AY8