

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111820\
 Data File : PD060113.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2020 13:48
 Operator : DD\AJ
 Sample : L4710-15
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0B44

Manual Integrations
 APPROVED

mohammad
 11/20/2020 1:50:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 06:04:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 04:05:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.504	4.023	9872284	39035779	11.520	13.095
27)	SA Decachlor...	8.299	9.104	10931452	29667361	13.156	12.060m
Target Compounds							
10)	B trans-Chl...	5.465	6.124	754117	15762039	0.710m	4.588 #
11)	B cis-Chlor...	5.522	6.213	947221	14896652	0.895m	4.339 #
12)	B 4,4'-DDE	5.688	6.363	1321868	9939719	1.293m	3.074 #
13)	MA Dieldrin	5.825	6.519	82914787	295.5E6	76.099	84.625
17)	MA 4,4'-DDT	6.448	7.158	4754337	15318235	5.290	5.629m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111820\
Data File : PD060113.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2020 13:48
Operator : DD\AJ
Sample : L4710-15
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 06:04:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

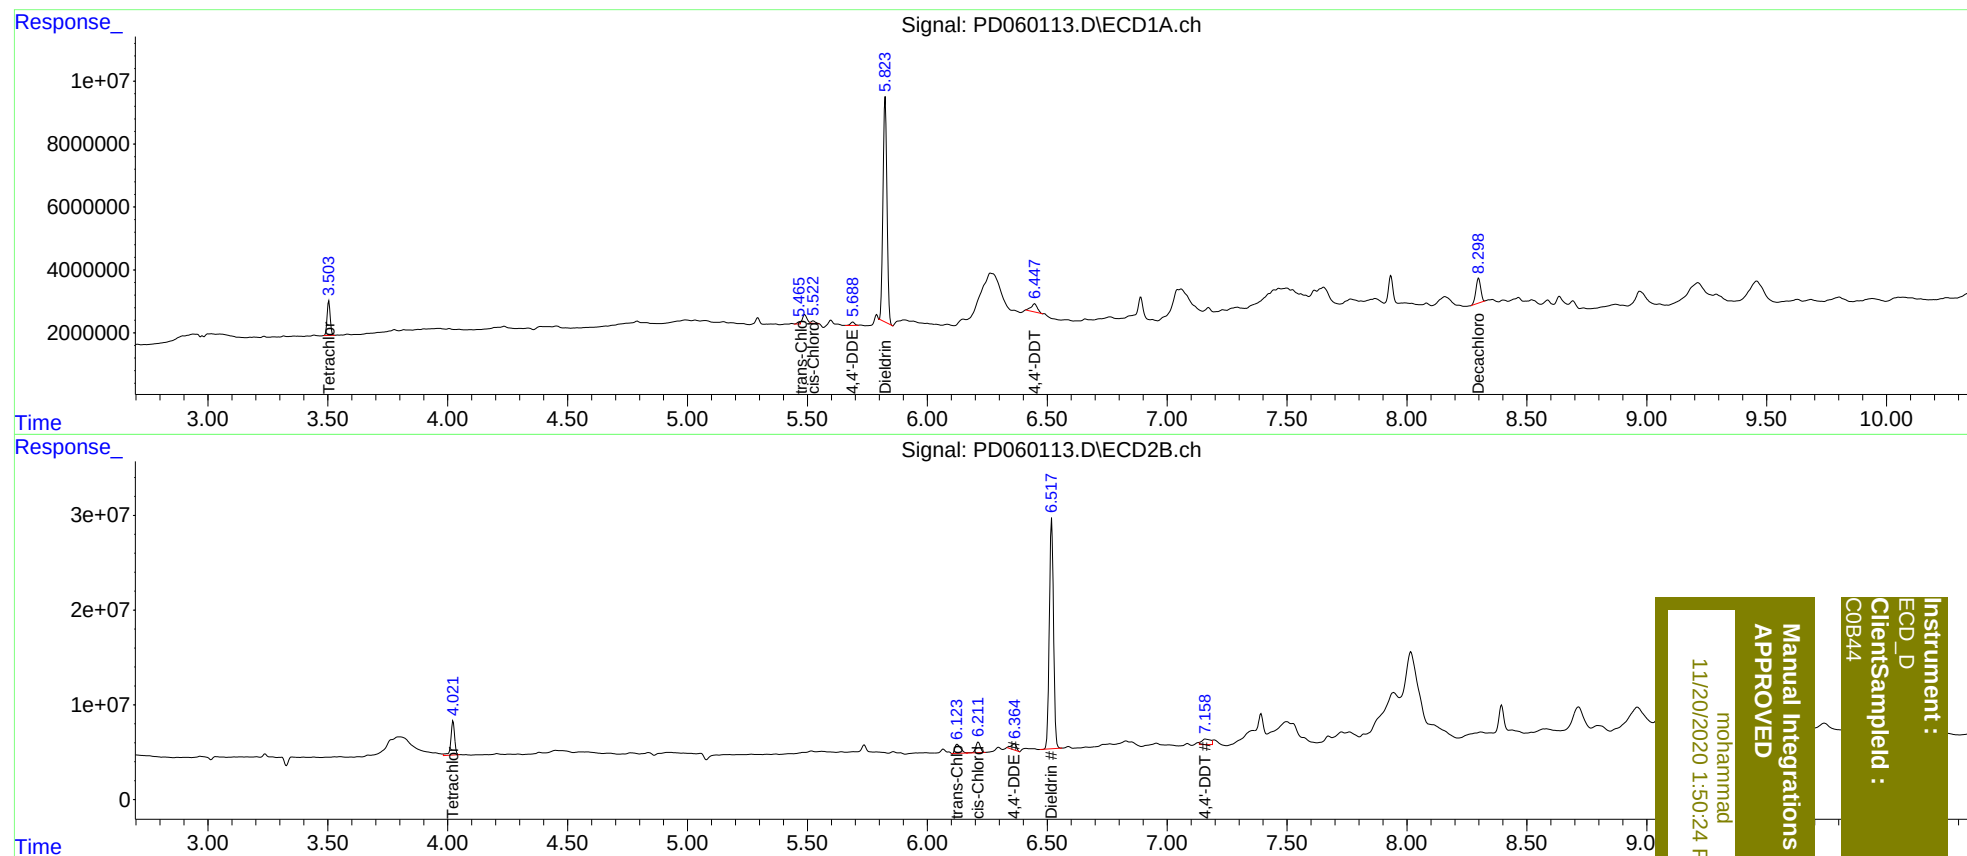

Manual Integrations
APPROVED

11/20/2020 1:50:24 PM
mohammad

Instrument :
ECD_D
ClientSampled :
C0B44