

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111820\
Data File : PD060099.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2020 10:16
Operator : DD\AJ
Sample : PB133023BS
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
PLCS23

Manual Integrations
APPROVED

Ankita
11/19/2020 1:20:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 05:58:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

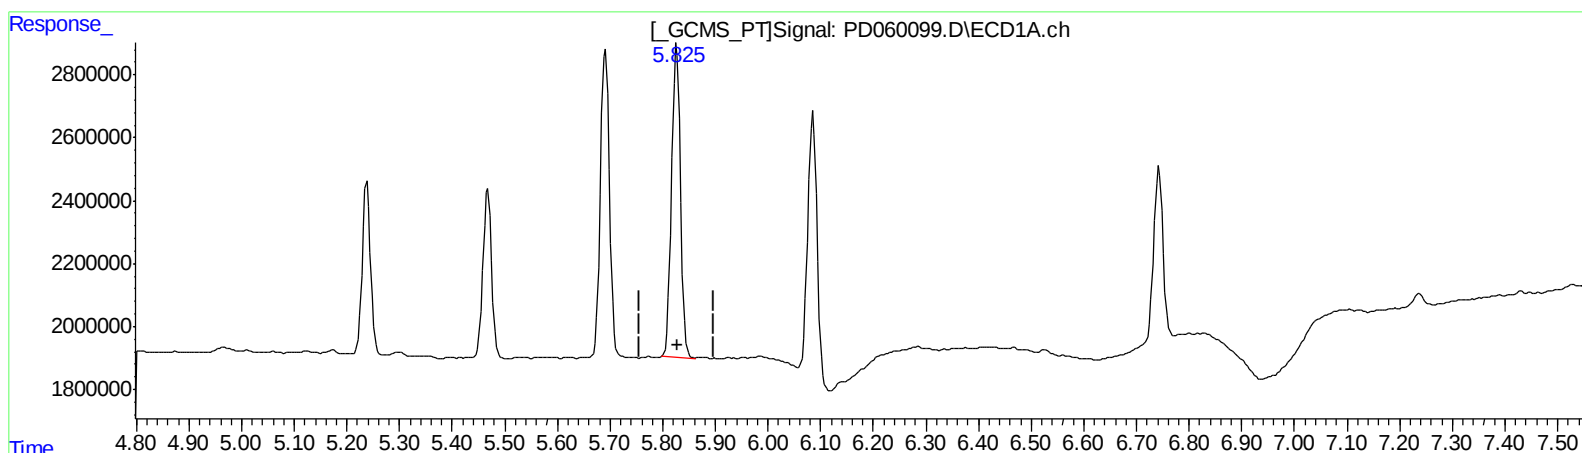

(13) Dieldrin (MA)
5.826min 10.749 ng/ml
response 11711875

(13) Dieldrin #2 (MA)
6.518min 10.693 ng/ml
response 37339967

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111820\
Data File : PD060099.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2020 10:16
Operator : DD\AJ
Sample : PB133023BS
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
PLCS23

Manual Integrations
APPROVED

Ankita
11/19/2020 1:20:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 05:58:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

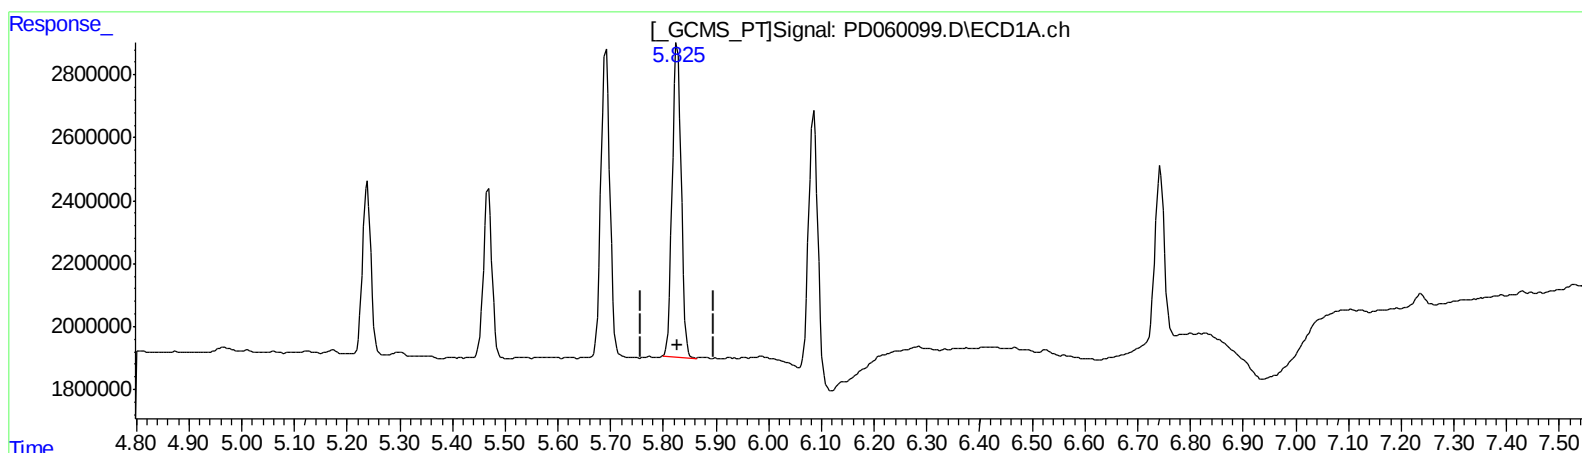

(13) Dieldrin (MA)
5.826min 10.749 ng/ml
response 11711875

(13) Dieldrin #2 (MA)
6.517min 10.700 ng/ml m
response 37363696

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111820\
 Data File : PD060099.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2020 10:16
 Operator : DD\AJ
 Sample : PB133023BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleID :
 PLCS23

Manual Integrations
 APPROVED

Ankita
 11/19/2020 1:20:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 05:58:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 04:05:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.505	4.022	17663122	65440069	20.611	21.953
27) SA Decachlor...	8.302	9.106	33067182	100.8E6	39.797	40.977
Target Compounds						
3) MA gamma-BHC...	4.233	4.698	5983747	18818661	4.895	4.650
8) B Heptachlo...	5.238	5.903	6115892	19034888	5.790	5.779
10) B trans-Chl...	5.468	6.137	6259478	19386187	5.893	5.643
12) B 4,4'-DDE	5.691	6.365	11711100	35008406	11.458	10.827
13) MA Dieldrin	5.826	6.517	11711875	37363696	10.749	10.700m
14) MA Endrin	6.085	6.736	10381074	30320907	11.507	10.829
19) B Endosulfa...	6.743	7.291	6819063	20782692	7.803	7.209

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

AJ
 11/24/20