

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111820\
 Data File : PD060105.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2020 11:56
 Operator : DD\AJ
 Sample : L4710-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AX2

Manual Integrations
 APPROVED

Ankita
 11/19/2020 1:20:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 06:00:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 04:05:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.505	4.023	11996558	44804593	13.999	15.031
27)	SA Decachlor...	8.296	9.105	27511124	74575354	33.111	30.315m
Target Compounds							
3)	MA gamma-BHC...	4.237	4.680	7402464	30706429	6.056	7.587 #
12)	B 4,4'-DDE	5.688	6.364	7991320	24788306	7.819m	7.666
15)	B Endosulfa...	6.364	6.954	5824166	30834632	6.459	10.908m#
16)	A 4,4'-DDD	6.207	6.854	1897356	25053629	2.145m	9.339 #
17)	MA 4,4'-DDT	6.451	7.156	7200534	26656960	8.012	9.796

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111820\
Data File : PD060105.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2020 11:56
Operator : DD\AJ
Sample : L4710-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 06:00:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

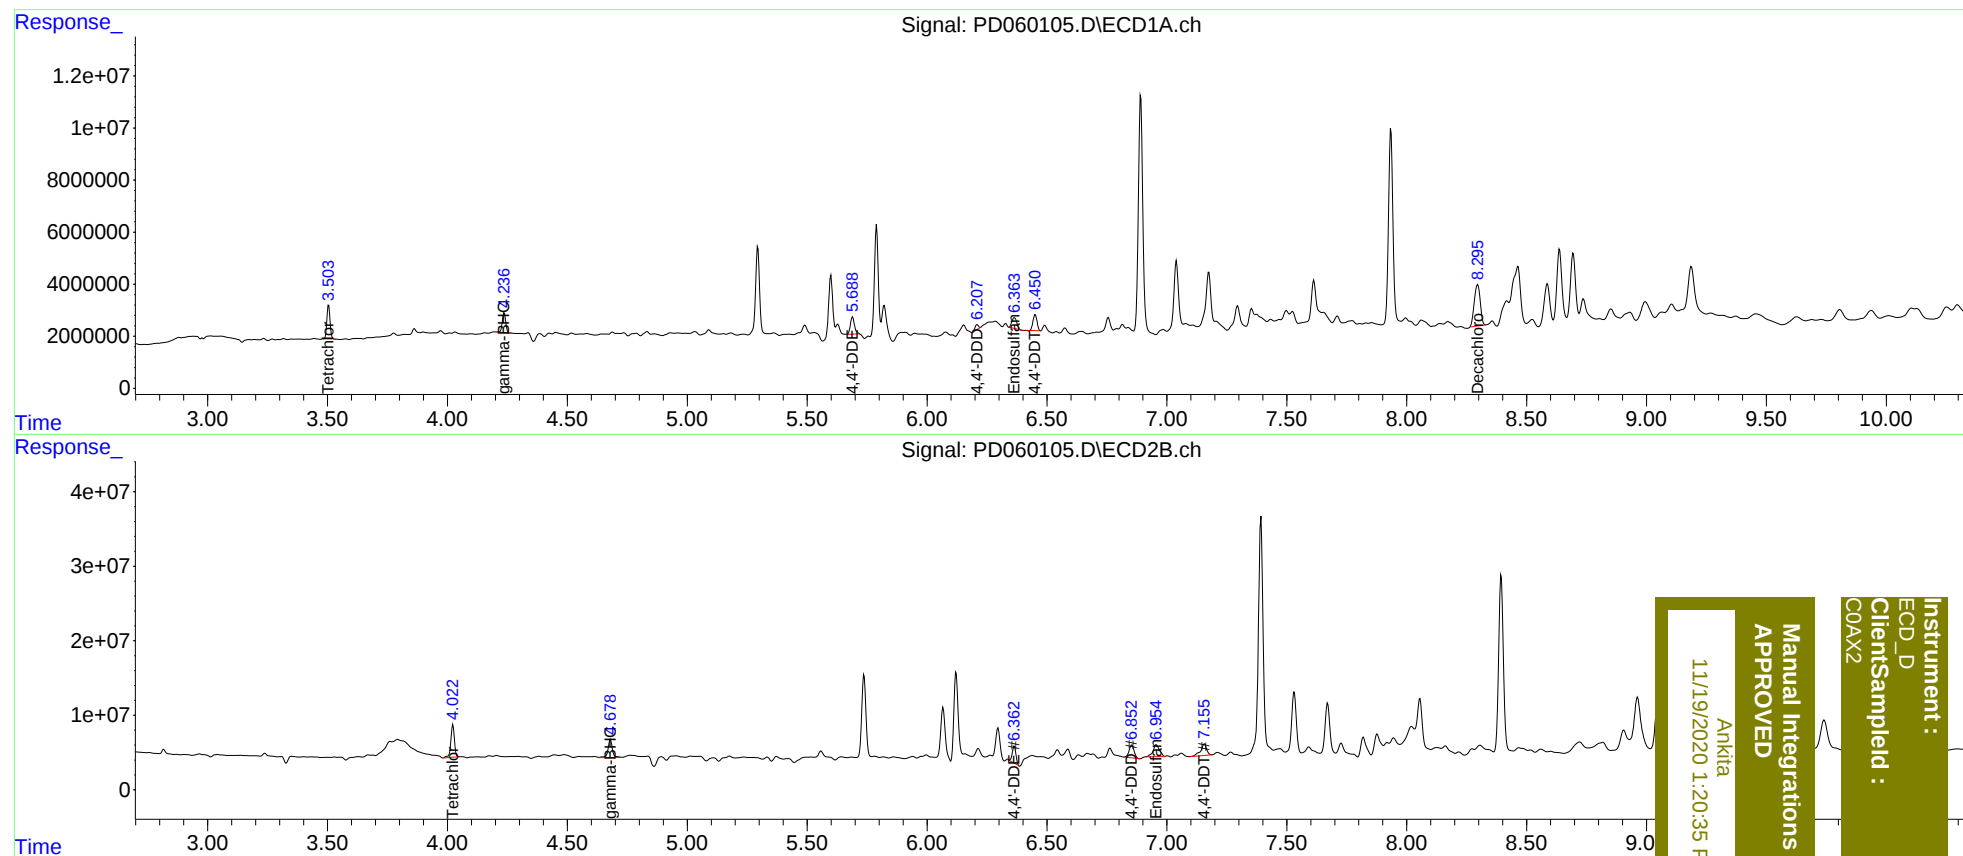

Manual Integrations
APPROVED

Ankita
11/19/2020 1:20:35 PM

Instrument :
ECD_D
ClientSampleId :
C0AX2