

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111822\
 Data File : PD073056.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2022 12:16
 Operator : AR\AJ
 Sample : PB148936BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 05:09:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.699	3.460	50208382	1355.5E6	20.938	20.750
2)	SA Decachlor...	7.829	8.912	95073793	625.8E6	41.665	42.287
Target Compounds							
2)	A alpha-BHC	0.000	3.928	0	14696533	N.D.	0.169
3)	MA gamma-BHC...	0.000	4.289f	0	4567084	N.D.	<MDL
4)	MA Heptachlor	0.000	4.832	0	1071072	N.D.	<MDL
5)	MB Aldrin	0.000	5.156	0	676766	N.D.	<MDL
6)	B beta-BHC	0.000	4.462	0	15904368	N.D.	0.595
7)	B delta-BHC	0.000	4.747f	0	11211911	N.D.	0.206
8)	B Heptachlo...	0.000	5.594	0	96683769	N.D.	2.860
9)	A Endosulfan I	0.000	5.988	0	1499173	N.D.	<MDL
11)	B cis-Chlor...	0.000	5.887f	0	8947838	N.D.	0.282
12)	B 4,4'-DDE	0.000	6.109	0	684866	N.D.	<MDL
13)	MA Dieldrin	0.000	6.258	0	15873328	N.D.	0.527
14)	MA Endrin	5.593	0.000	250617	0	<MDL	N.D. #
15)	B Endosulfa...	5.880	6.757f	190244	-524823	<MDL	N.D. #
16)	A 4,4'-DDD	0.000	6.627	0	1540433	N.D.	<MDL
17)	MA 4,4'-DDT	0.000	6.904	0	197388	N.D.	<MDL
19)	B Endosulfa...	0.000	7.040f	0	438590	N.D.	<MDL
20)	A Methoxychlor	0.000	7.340f	0	5004824	N.D.	0.536
22)	Toxaphene-1	0.000	5.764	0	20236908	N.D.	172.217
23)	Toxaphene-2	5.593	6.109f	250617	684866	16.027	3.196 #
24)	Toxaphene-3	5.880	6.904f	190244	197388	8.851	0.393 #
25)	Toxaphene-4	0.000	7.040	0	438590	N.D.	0.982


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111822\
Data File : PD073056.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2022 12:16
Operator : AR\AJ
Sample : PB148936BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 05:09:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

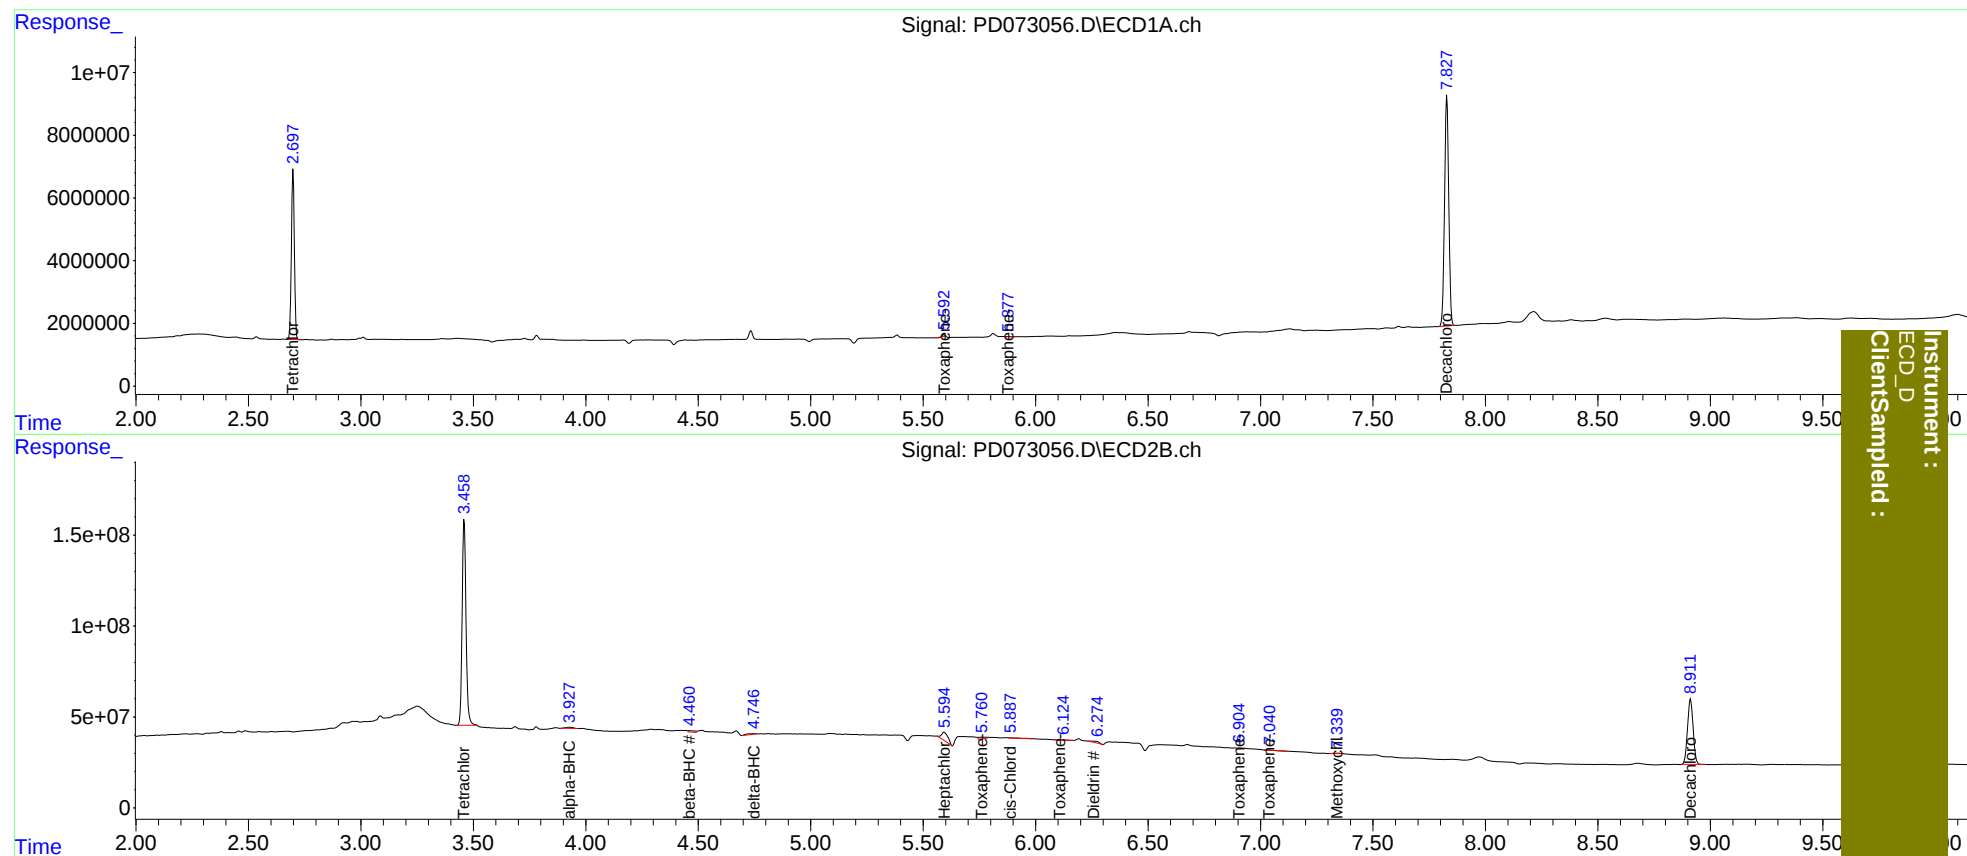


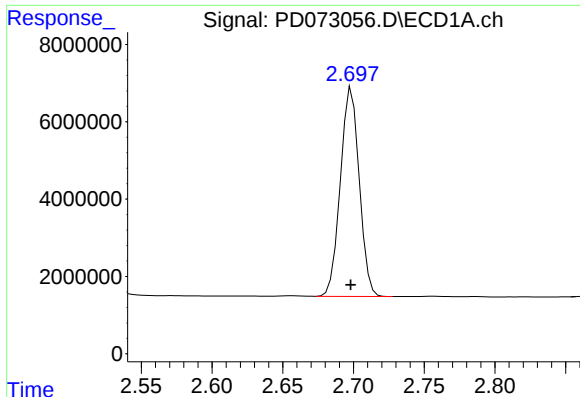

#1 Tetrachloro-m-xylene


R.T.: 2.699 min
Delta R.T.: 0.000 min
Response: 50208382
Conc: 20.94 ng/ml

Instrument :
ECD_D
ClientSampleId :

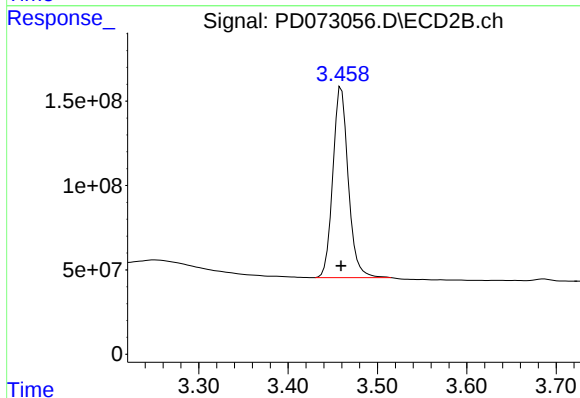


#1 Tetrachloro-m-xylene

R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 1355455140
Conc: 20.75 ng/ml

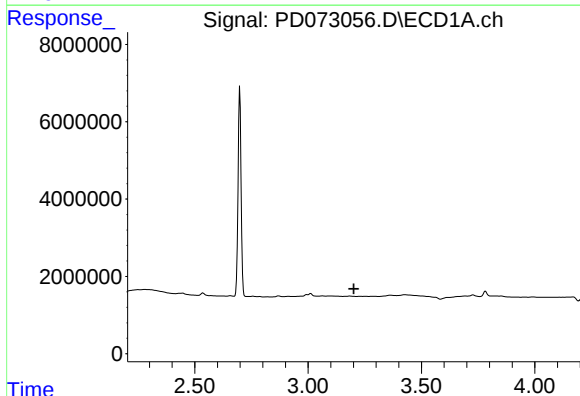


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.201 min
Response: 0
Conc: N.D.

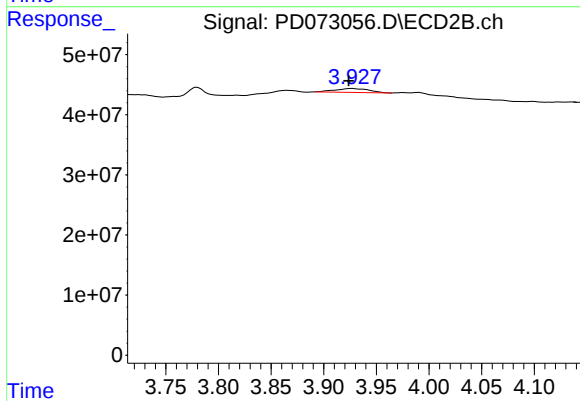

#2 alpha-BHC


R.T.: 3.928 min
Delta R.T.: 0.004 min
Response: 14696533
Conc: 0.17 ng/ml

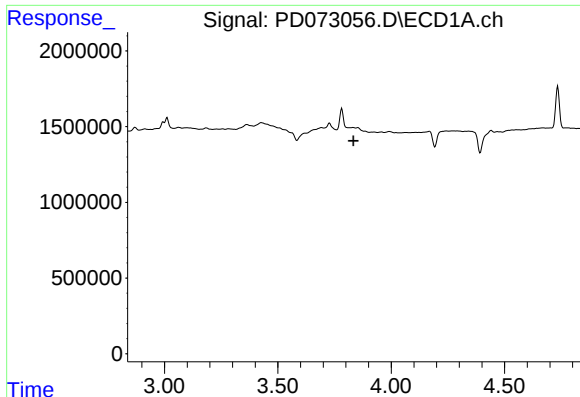

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 3.834 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

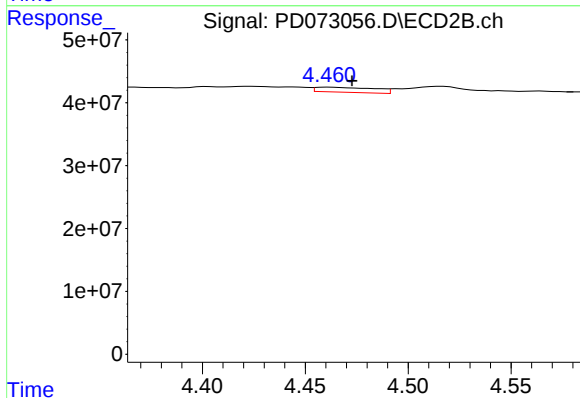


#6 beta-BHC

R.T.: 4.462 min
Delta R.T.: -0.011 min
Response: 15904368
Conc: 0.60 ng/ml

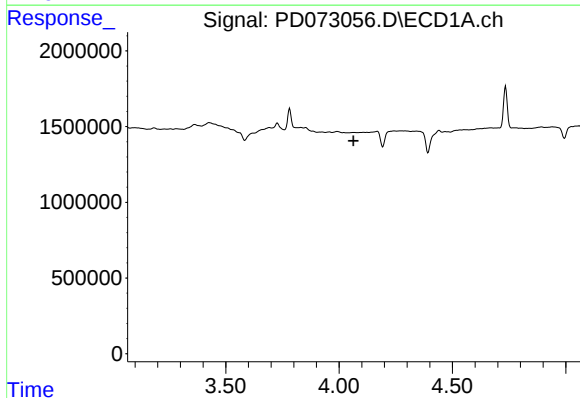


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.064 min
Response: 0
Conc: N.D.

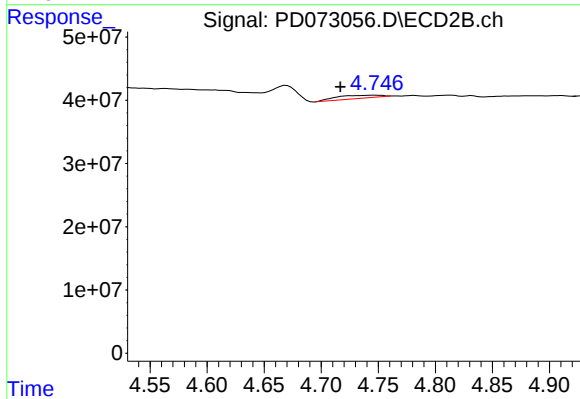

#7 delta-BHC


R.T.: 4.747 min
Delta R.T.: 0.031 min
Response: 11211911
Conc: 0.21 ng/ml

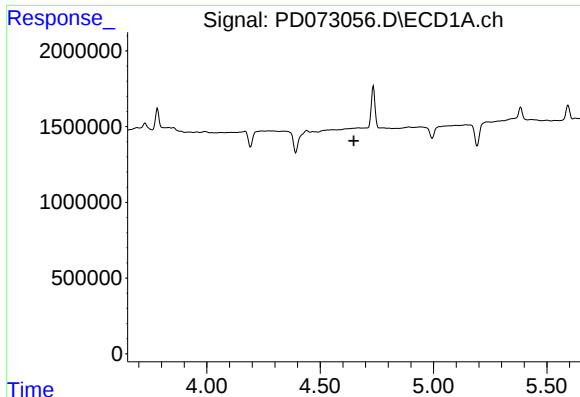

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.649 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

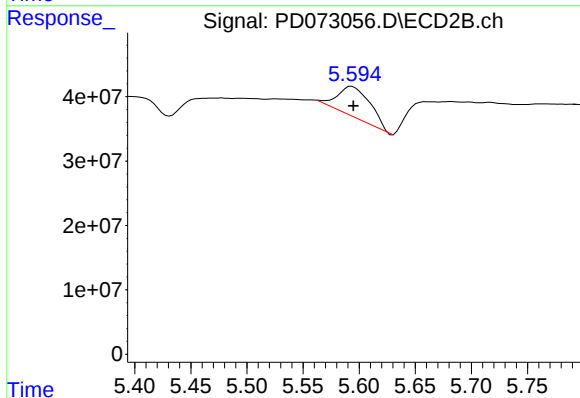


#8 Heptachlor epoxide

R.T.: 5.594 min
Delta R.T.: -0.001 min
Response: 96683769
Conc: 2.86 ng/ml

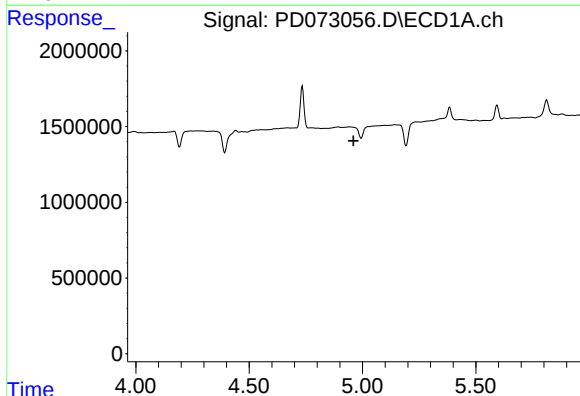


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 4.961 min
Response: 0
Conc: N.D.

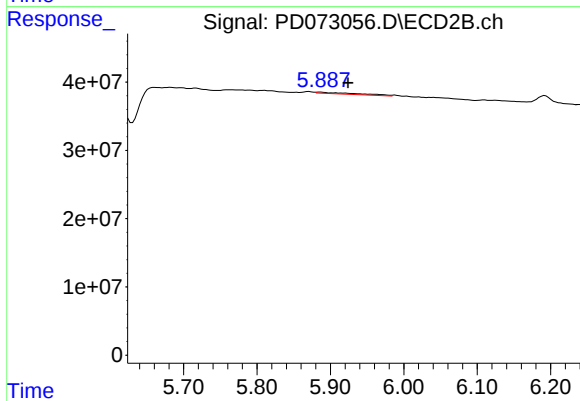

#11 cis-Chlordane


R.T.: 5.887 min
Delta R.T.: -0.037 min
Response: 8947838
Conc: 0.28 ng/ml

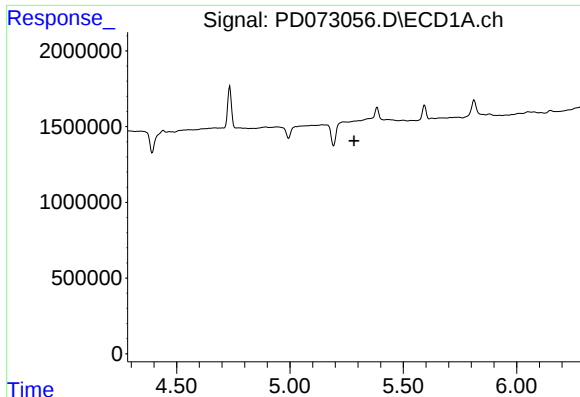

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

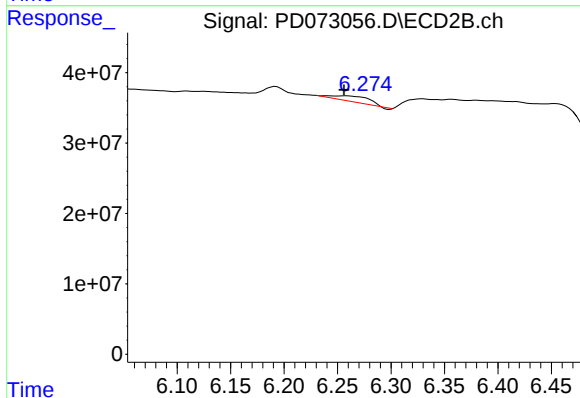


#13 Dieldrin

R.T.: 6.258 min
Delta R.T.: 0.002 min
Response: 15873328
Conc: 0.53 ng/ml

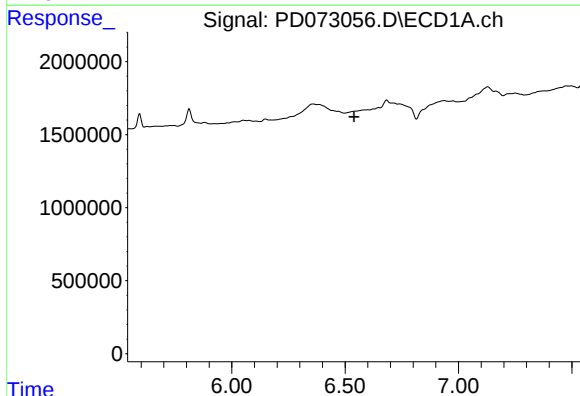


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.539 min
Response: 0
Conc: N.D.

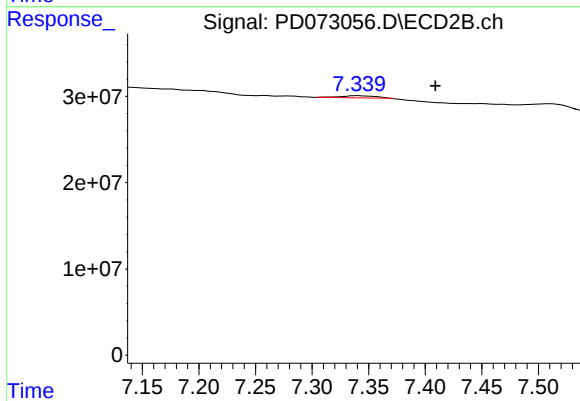

#20 Methoxychlor


R.T.: 7.340 min
Delta R.T.: -0.069 min
Response: 5004824
Conc: 0.54 ng/ml

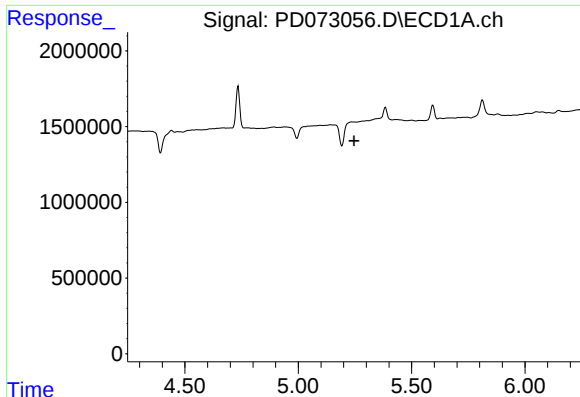

#22 Toxaphene-1


R.T.: 0.000 min
Exp R.T.: 5.246 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

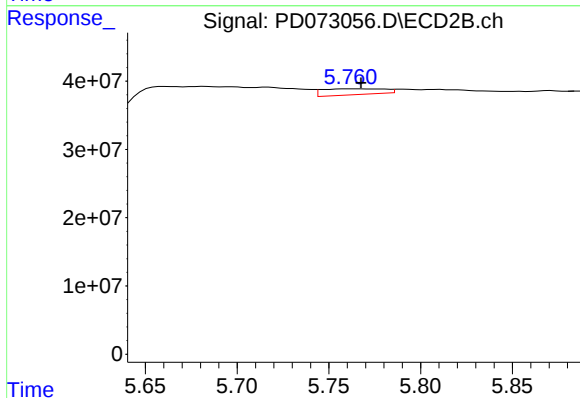


#22 Toxaphene-1

R.T.: 5.764 min
Delta R.T.: -0.004 min
Response: 20236908
Conc: 172.22 ng/ml

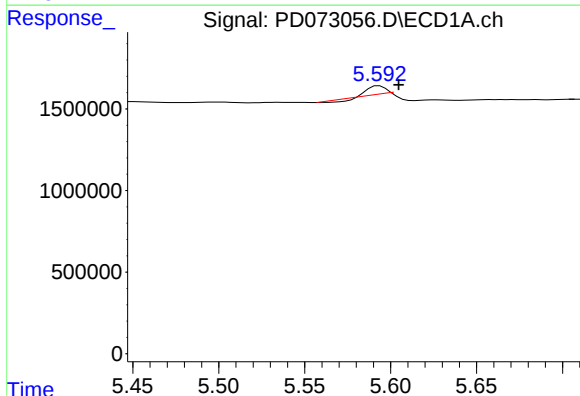


#23 Toxaphene-2

R.T.: 5.593 min
Delta R.T.: -0.011 min
Response: 250617
Conc: 16.03 ng/ml

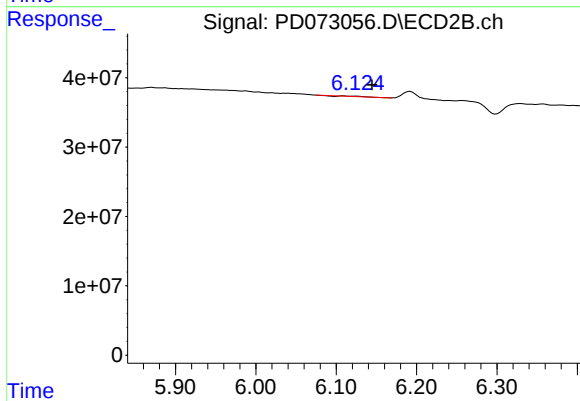

#23 Toxaphene-2


R.T.: 6.109 min
Delta R.T.: -0.035 min
Response: 684866
Conc: 3.20 ng/ml

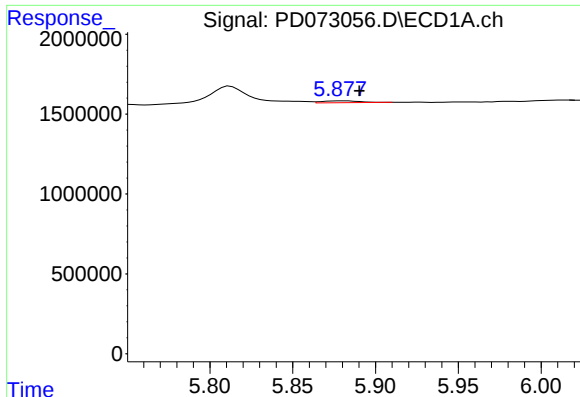

#24 Toxaphene-3


R.T.: 5.880 min
Delta R.T.: -0.010 min
Response: 190244
Conc: 8.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

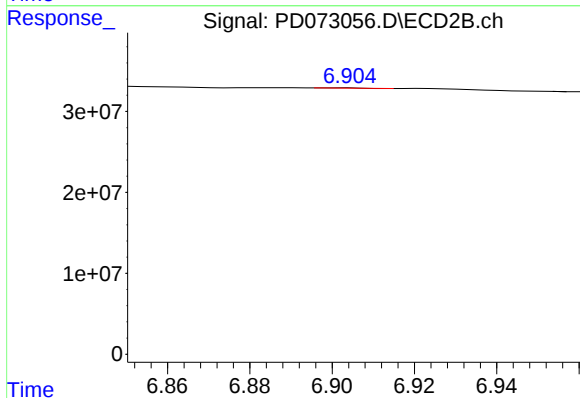


#24 Toxaphene-3

R.T.: 6.904 min
Delta R.T.: -0.063 min
Response: 197388
Conc: 0.39 ng/ml

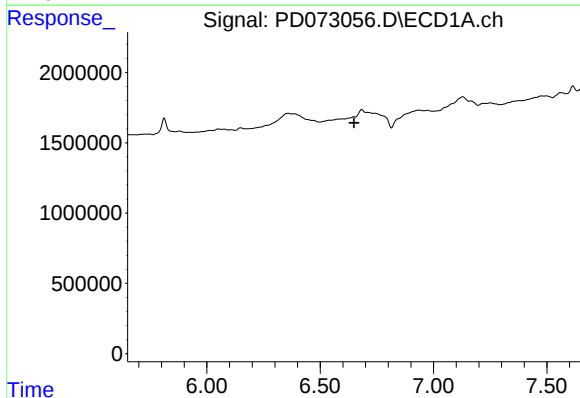


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T. : 6.649 min
Response: 0
Conc: N.D.

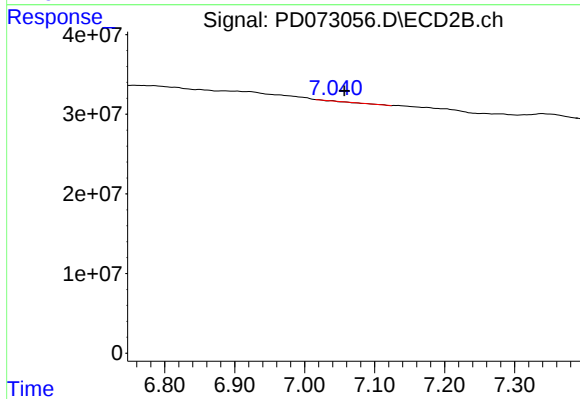

#25 Toxaphene-4


R.T.: 7.040 min
Delta R.T.: -0.017 min
Response: 438590
Conc: 0.98 ng/ml

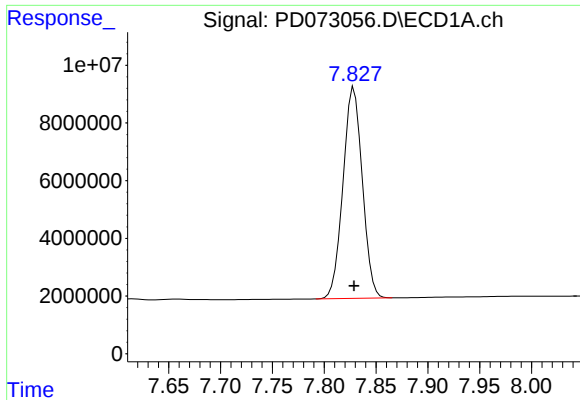

#27 Decachlorobiphenyl

R.T.: 7.829 min
Delta R.T.: 0.000 min
Response: 95073793
Conc: 41.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

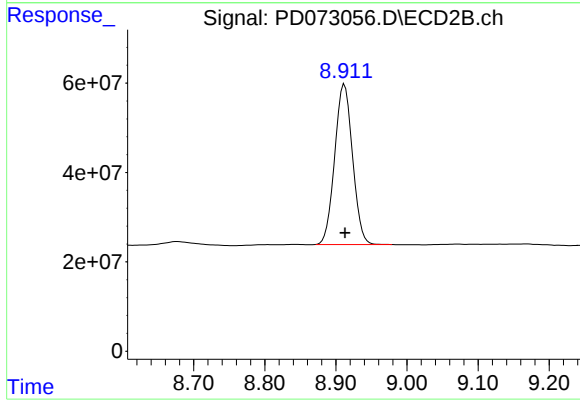

#27 Decachlorobiphenyl

R.T.: 8.912 min
Delta R.T.: 0.000 min
Response: 625779835
Conc: 42.29 ng/ml