

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111822\
 Data File : PD073068.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2022 15:00
 Operator : AR\AJ
 Sample : N5574-02MS
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 B0AA0MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 05:12:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.699	3.462	45600537	1505.7E6	19.016	23.049
2)	SA Decachlor...	7.828	8.912	77036393	495.0E6	33.760	33.451
Target Compounds							
2)	A alpha-BHC	3.202	3.924	161.7E6	3260.8E6	44.178	37.392
3)	MA gamma-BHC...	3.532	4.258	160.6E6	2712.0E6	48.385	39.970
4)	MA Heptachlor	3.864	4.824	161.4E6	1862.3E6	48.325	40.554
5)	MB Aldrin	4.143	5.162	159.6E6	1612.7E6	47.371	40.156
6)	B beta-BHC	3.834	4.473	74462035	1228.7E6	46.378	45.988
7)	B delta-BHC	4.063	4.716	12194436	225.5E6	3.355	4.145
8)	B Heptachlo...	4.648	5.594	155.2E6	1490.5E6	49.954	44.096
9)	A Endosulfan I	5.017	5.979	142.0E6	1320.7E6	50.231	45.401
10)	B trans-Chl...	4.897	5.848	150.4E6	1362.2E6	48.806	43.121
11)	B cis-Chlor...	4.960	5.923	145.8E6	1338.8E6	46.560	42.172
12)	B 4,4'-DDE	5.148	6.097	295.7E6	2596.1E6	98.844	86.470
13)	MA Dieldrin	5.283	6.256	325.3E6	2833.8E6	106.195	94.012
14)	MA Endrin	5.560	6.487	286.2E6	2252.2E6	105.578	91.305
15)	B Endosulfa...	5.858	6.717	271.4E6	2235.6E6	100.795	92.541
16)	A 4,4'-DDD	5.707	6.622	236.6E6	2010.7E6	98.195	87.735
17)	MA 4,4'-DDT	5.955	6.930	232.1E6	1984.5E6	103.756	92.401
18)	B Endrin al...	6.040	6.848	197.4E6	1612.6E6	91.418	85.121
19)	B Endosulfa...	6.263	7.081	163.6E6	1297.4E6	65.204	62.391
20)	A Methoxychlor	6.539	7.409	644.7E6	4452.9E6	514.761	477.248
21)	B Endrin ke...	6.773	7.571	304.7E6	2149.9E6	104.392	96.289

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111822\
Data File : PD073068.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2022 15:00
Operator : AR\AJ
Sample : N5574-02MS
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 05:12:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

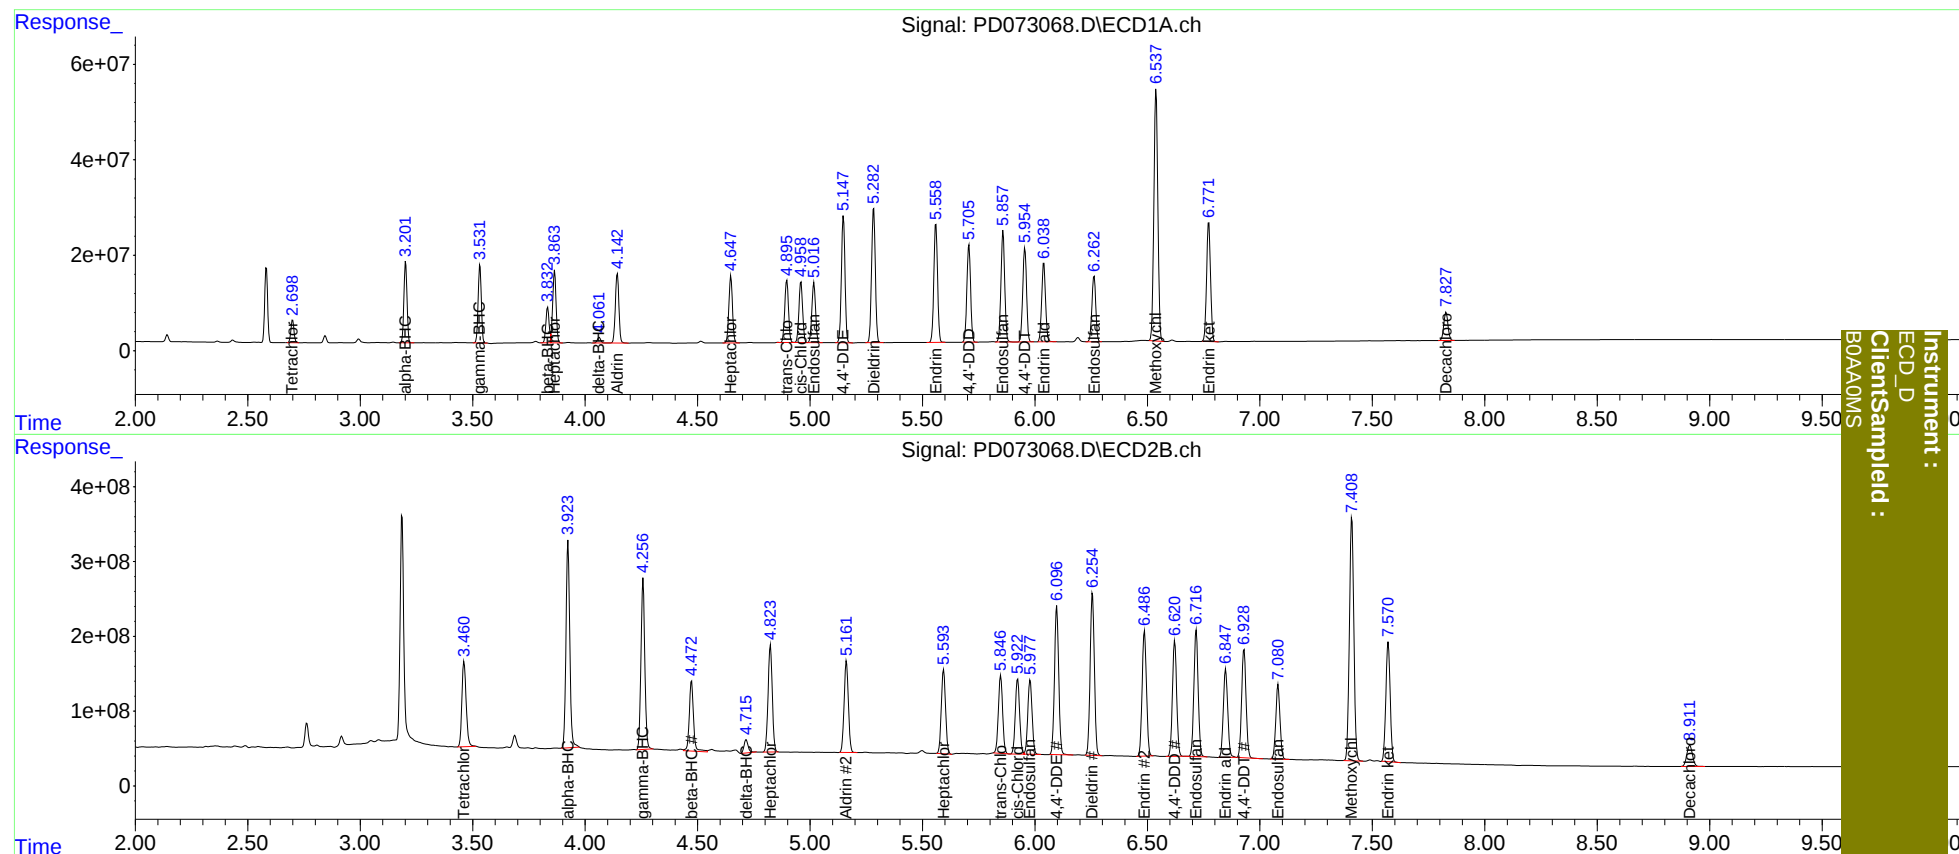

Instrument :
ECD_D
ClientSampled :
BOA0A0MS