

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111822\
 Data File : PD073073.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2022 16:17
 Operator : AR\AJ
 Sample : PB149089BS
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS089

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 05:13:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.699	3.460	44988173	1192.7E6	18.761	18.258
2)	SA Decachlor...	7.829	8.912	85690847	551.8E6	37.553	37.289
Target Compounds							
2)	A alpha-BHC	3.202	3.924	16130709	423.0E6	4.408	4.851
3)	MA gamma-BHC...	3.532	4.257	14934629	344.1E6	4.500	5.071
4)	MA Heptachlor	3.864	4.824	15382232	226.3E6	4.604	4.928
5)	MB Aldrin	4.143	5.162	15920610	207.4E6	4.725	5.164
6)	B beta-BHC	3.834	4.472	8007267	149.8E6	4.987	5.607
7)	B delta-BHC	4.063	4.716	15350999	273.3E6	4.224	5.023
8)	B Heptachlo...	4.648	5.595	14636865	166.1E6	4.711	4.913
9)	A Endosulfan I	5.017	5.979	13512546	143.2E6	4.781	4.922
10)	B trans-Chl...	4.896	5.848	14619513	150.2E6	4.743	4.754
11)	B cis-Chlor...	4.959	5.923	14634449	151.9E6	4.674	4.784
12)	B 4,4'-DDE	5.148	6.097	25697391	286.1E6	8.590	9.530
13)	MA Dieldrin	5.283	6.256	27861671	296.9E6	9.095	9.850
14)	MA Endrin	5.560	6.488	24736055	241.1E6	9.124	9.775
15)	B Endosulfa...	5.858	6.717	24958407	235.1E6	9.268	9.730
16)	A 4,4'-DDD	5.706	6.621	22668114	234.1E6	9.409	10.216
17)	MA 4,4'-DDT	5.955	6.929	20456376	209.5E6	9.145	9.754
18)	B Endrin al...	6.040	6.849	20650936	174.3E6	9.561	9.203
19)	B Endosulfa...	6.263	7.082	23348848	200.4E6	9.306	9.638
20)	A Methoxychlor	6.539	7.410	61045332	477.6E6	48.740	51.187
21)	B Endrin ke...	6.774	7.571	28402108	233.6E6	9.730	10.462

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111822\
Data File : PD073073.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2022 16:17
Operator : AR\AJ
Sample : PB149089BS
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 05:13:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

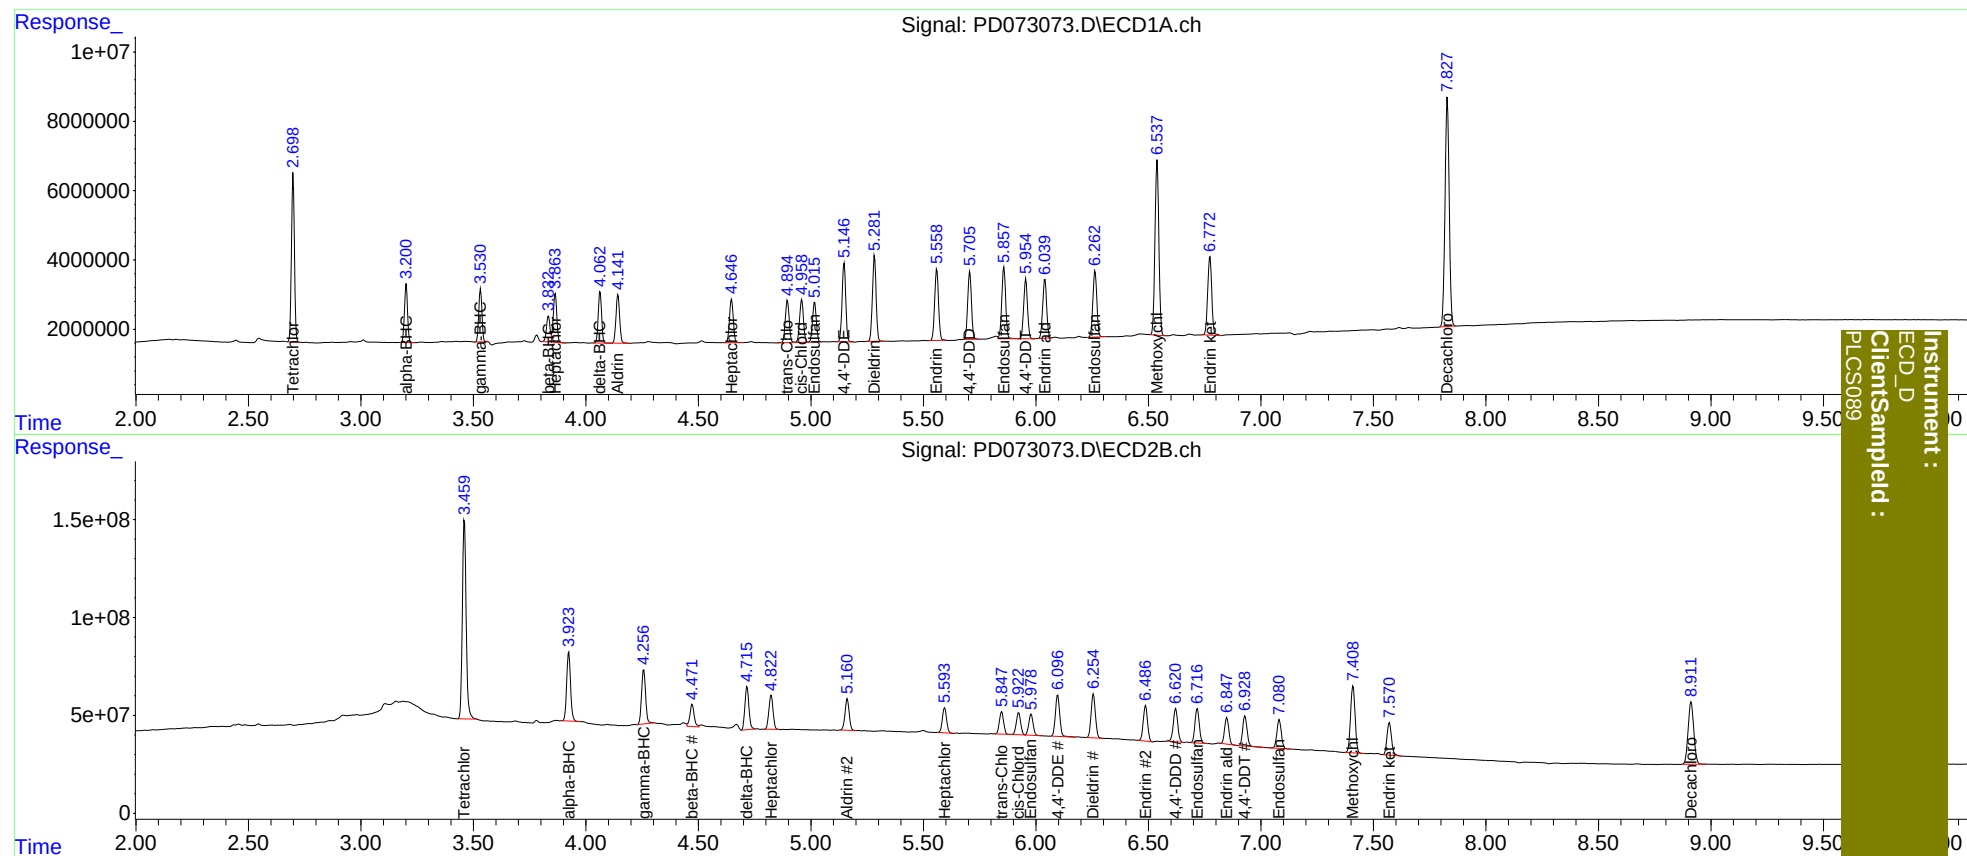

Instrument :
ECD_D
ClientSampled :
PLCS089