

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111822\
 Data File : PD073058.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2022 12:43
 Operator : AR\AJ
 Sample : N5407-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW4Y1

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/21/2022
 Supervised By : Ankita Jodhani 11/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 05:09:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	2.702	3.457	48304073	1854.5E6	20.144	28.389 #
2) SA Decachlor...	7.828	8.912	32312343	252.7E6	14.160m	17.074
Target Compounds						
16) A 4,4'-DDD	5.724	6.638	9035052	131.2E6	3.750m	5.723 #
18) B Endrin al...	6.020	6.847	26344675	67906946	12.198m	3.585m#
20) A Methoxychlor	6.535	7.410	18093503	55442898	14.446m	5.942m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111822\
Data File : PD073058.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2022 12:43
Operator : AR\AJ
Sample : N5407-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 05:09:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

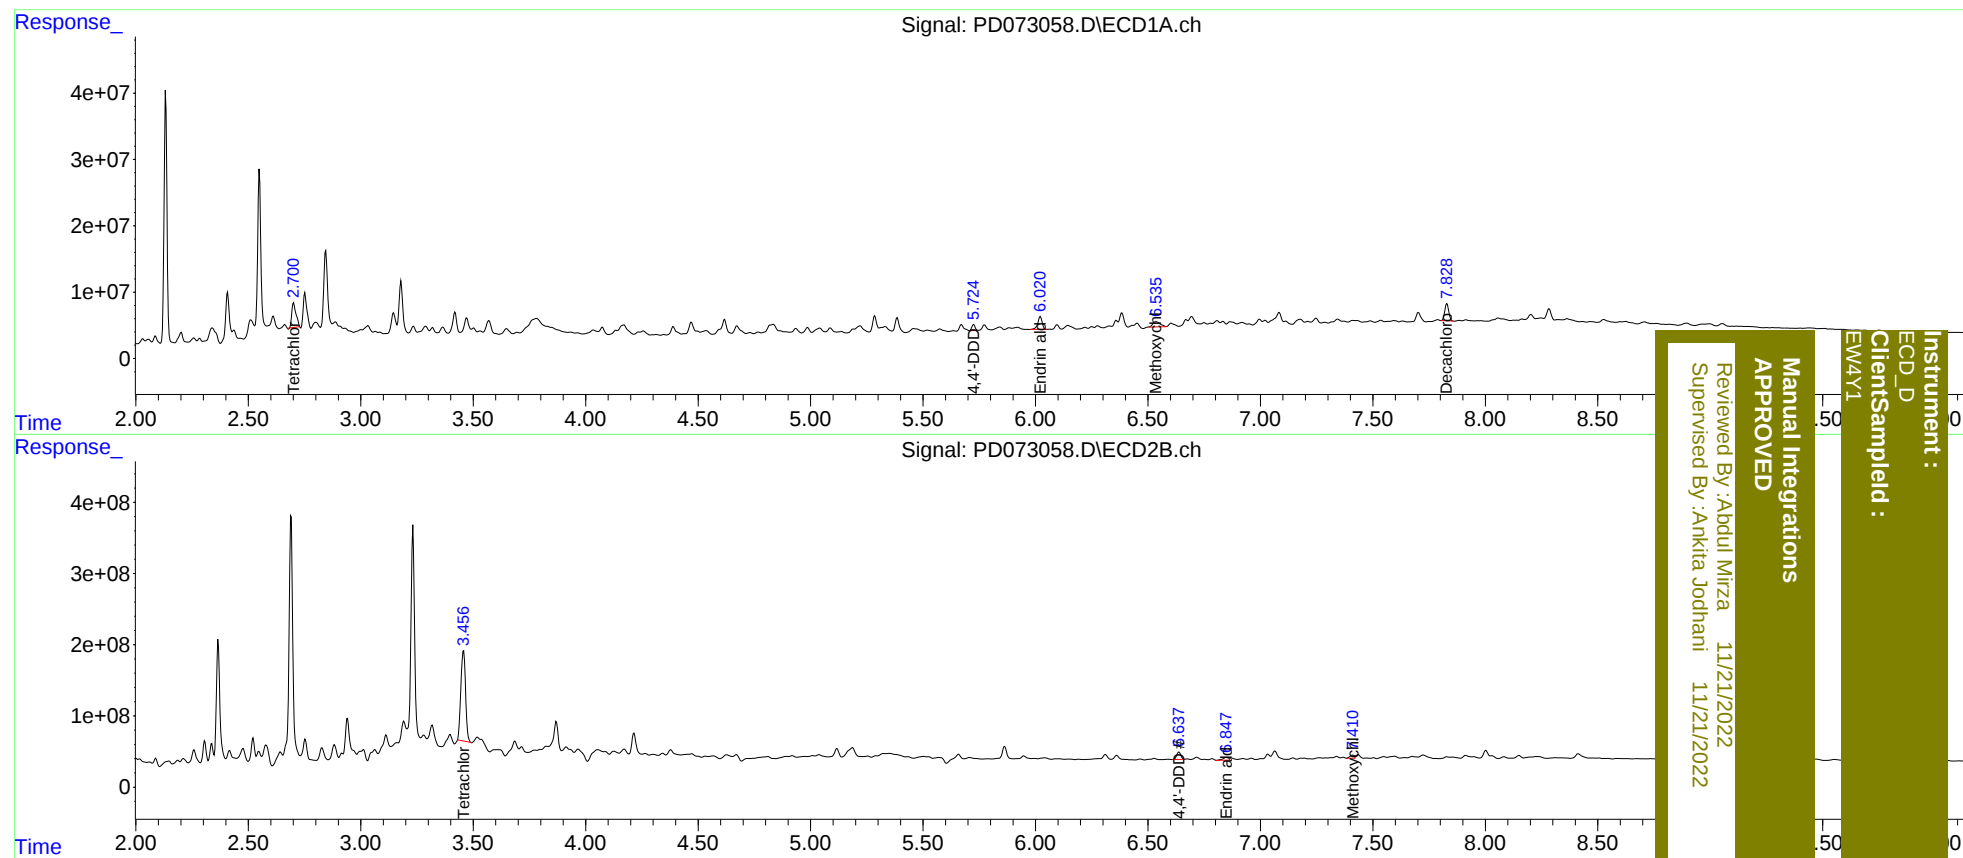

Instrument :
ECD_D
ClientSampled :
EW4Y1
Manual Integrations
APPROVED
Reviewed By :Abdul Mirza 11/21/2022
Supervised By :Ankita Jodhani 11/21/2022