

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111822\
 Data File : PD073062.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2022 13:40
 Operator : AR\AJ
 Sample : N5541-02MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0KX8MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 05:10:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.699	3.462	42196870	1404.3E6	17.597	21.497
2)	SA Decachlor...	7.829	8.912	73814203	479.6E6	32.348	32.408
Target Compounds							
2)	A alpha-BHC	3.202	3.924	147.1E6	2995.6E6	40.197	34.351
3)	MA gamma-BHC...	3.532	4.258	144.9E6	2491.7E6	43.661	36.723
4)	MA Heptachlor	3.865	4.824	144.2E6	1649.1E6	43.160	35.912
5)	MB Aldrin	4.143	5.163	145.5E6	1486.9E6	43.172	37.024
6)	B beta-BHC	3.834	4.473	67487285	1101.4E6	42.034	41.223
7)	B delta-BHC	4.063	4.717	12472480	207.0E6	3.432	3.805
8)	B Heptachlo...	4.649	5.595	139.8E6	1341.2E6	44.986	39.677
9)	A Endosulfan I	5.018	5.979	128.5E6	1192.3E6	45.478	40.988
10)	B trans-Chl...	4.897	5.849	140.0E6	1252.5E6	45.408	39.649
11)	B cis-Chlor...	4.961	5.924	134.8E6	1230.1E6	43.039	38.746
12)	B 4,4'-DDE	5.149	6.097	279.4E6	2453.9E6	93.400	81.736
13)	MA Dieldrin	5.283	6.256	294.3E6	2549.2E6	96.064	84.569
14)	MA Endrin	5.560	6.488	257.4E6	2030.4E6	94.962	82.312
15)	B Endosulfa...	5.859	6.718	241.6E6	1980.7E6	89.701	81.990
16)	A 4,4'-DDD	5.707	6.622	216.5E6	1849.5E6	89.863	80.701
17)	MA 4,4'-DDT	5.956	6.930	208.3E6	1801.8E6	93.126	83.894
18)	B Endrin al...	6.041	6.849	175.4E6	1433.0E6	81.223	75.643
19)	B Endosulfa...	6.264	7.082	148.1E6	1169.2E6	59.022	56.225
20)	A Methoxychlor	6.540	7.409	576.6E6	3970.3E6	460.363	425.525
21)	B Endrin ke...	6.774	7.571	272.4E6	1908.1E6	93.302	85.460

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111822\
Data File : PD073062.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2022 13:40
Operator : AR\AJ
Sample : N5541-02MS
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 05:10:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

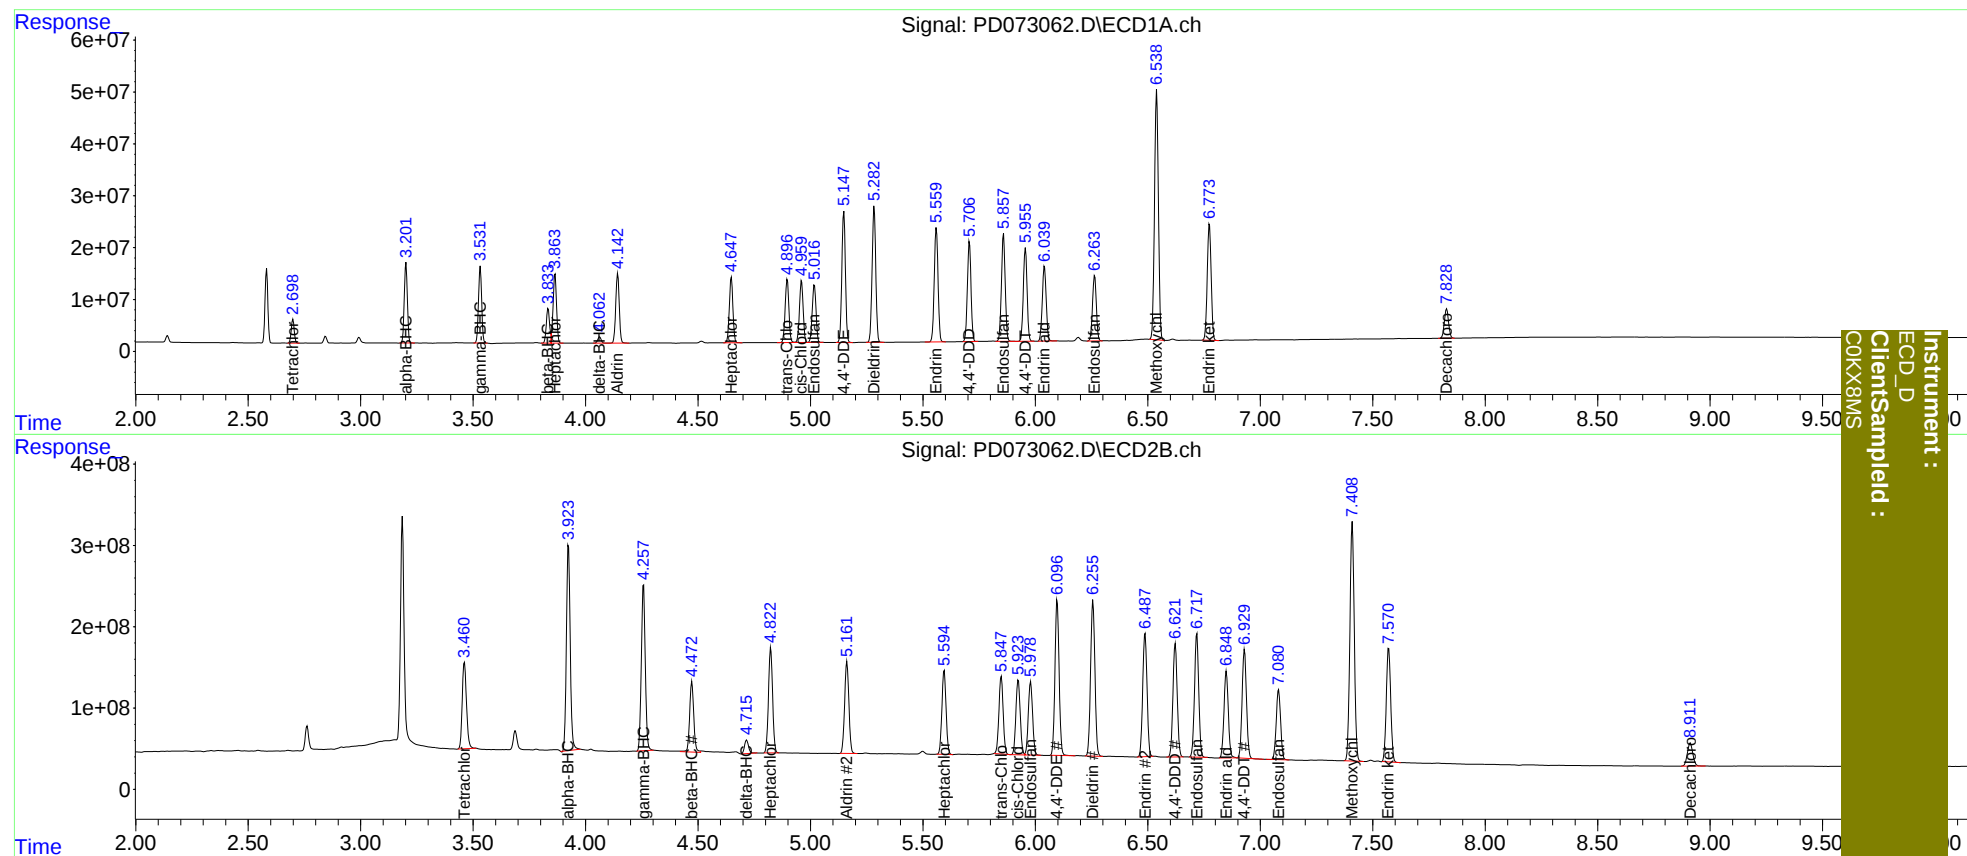

Instrument :
ECD_D
ClientSampled :
C0KX8MS