

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111822\
 Data File : PD073063.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2022 13:53
 Operator : AR\AJ
 Sample : N5541-03MSD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0KX8MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 05:10:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.699	3.461	42706685	1444.2E6	17.810	22.108
27)	SA Decachlor...	7.829	8.912	75128547	486.4E6	32.924	32.872
Target Compounds							
2)	A alpha-BHC	3.202	3.924	148.4E6	3058.1E6	40.545	35.068
3)	MA gamma-BHC...	3.532	4.257	146.2E6	2523.9E6	44.064	37.198
4)	MA Heptachlor	3.864	4.824	145.4E6	1674.3E6	43.525	36.461
5)	MB Aldrin	4.144	5.162	146.8E6	1500.4E6	43.557	37.361
6)	B beta-BHC	3.834	4.473	68151167	1150.1E6	42.448	43.046
7)	B delta-BHC	4.063	4.716	12683487	209.5E6	3.490	3.850
8)	B Heptachlo...	4.648	5.594	141.5E6	1357.1E6	45.553	40.149
9)	A Endosulfan I	5.017	5.979	130.3E6	1213.7E6	46.112	41.722
10)	B trans-Chl...	4.896	5.848	141.7E6	1273.5E6	45.980	40.312
11)	B cis-Chlor...	4.960	5.924	137.0E6	1252.4E6	43.750	39.449
12)	B 4,4'-DDE	5.149	6.097	282.9E6	2498.3E6	94.578	83.216
13)	MA Dieldrin	5.283	6.256	297.7E6	2585.3E6	97.186	85.768
14)	MA Endrin	5.560	6.488	260.3E6	2081.0E6	96.015	84.364
15)	B Endosulfa...	5.859	6.717	245.5E6	2018.8E6	91.173	83.567
16)	A 4,4'-DDD	5.707	6.622	220.4E6	1875.9E6	91.477	81.853
17)	MA 4,4'-DDT	5.956	6.930	210.4E6	1826.9E6	94.043	85.064
18)	B Endrin al...	6.041	6.849	178.5E6	1456.6E6	82.625	76.888
19)	B Endosulfa...	6.263	7.082	150.7E6	1189.5E6	60.065	57.202
20)	A Methoxychlor	6.539	7.410	582.0E6	4020.6E6	464.709	430.912
21)	B Endrin ke...	6.774	7.571	277.0E6	1945.5E6	94.875	87.135

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111822\
Data File : PD073063.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2022 13:53
Operator : AR\AJ
Sample : N5541-03MSD
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 05:10:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

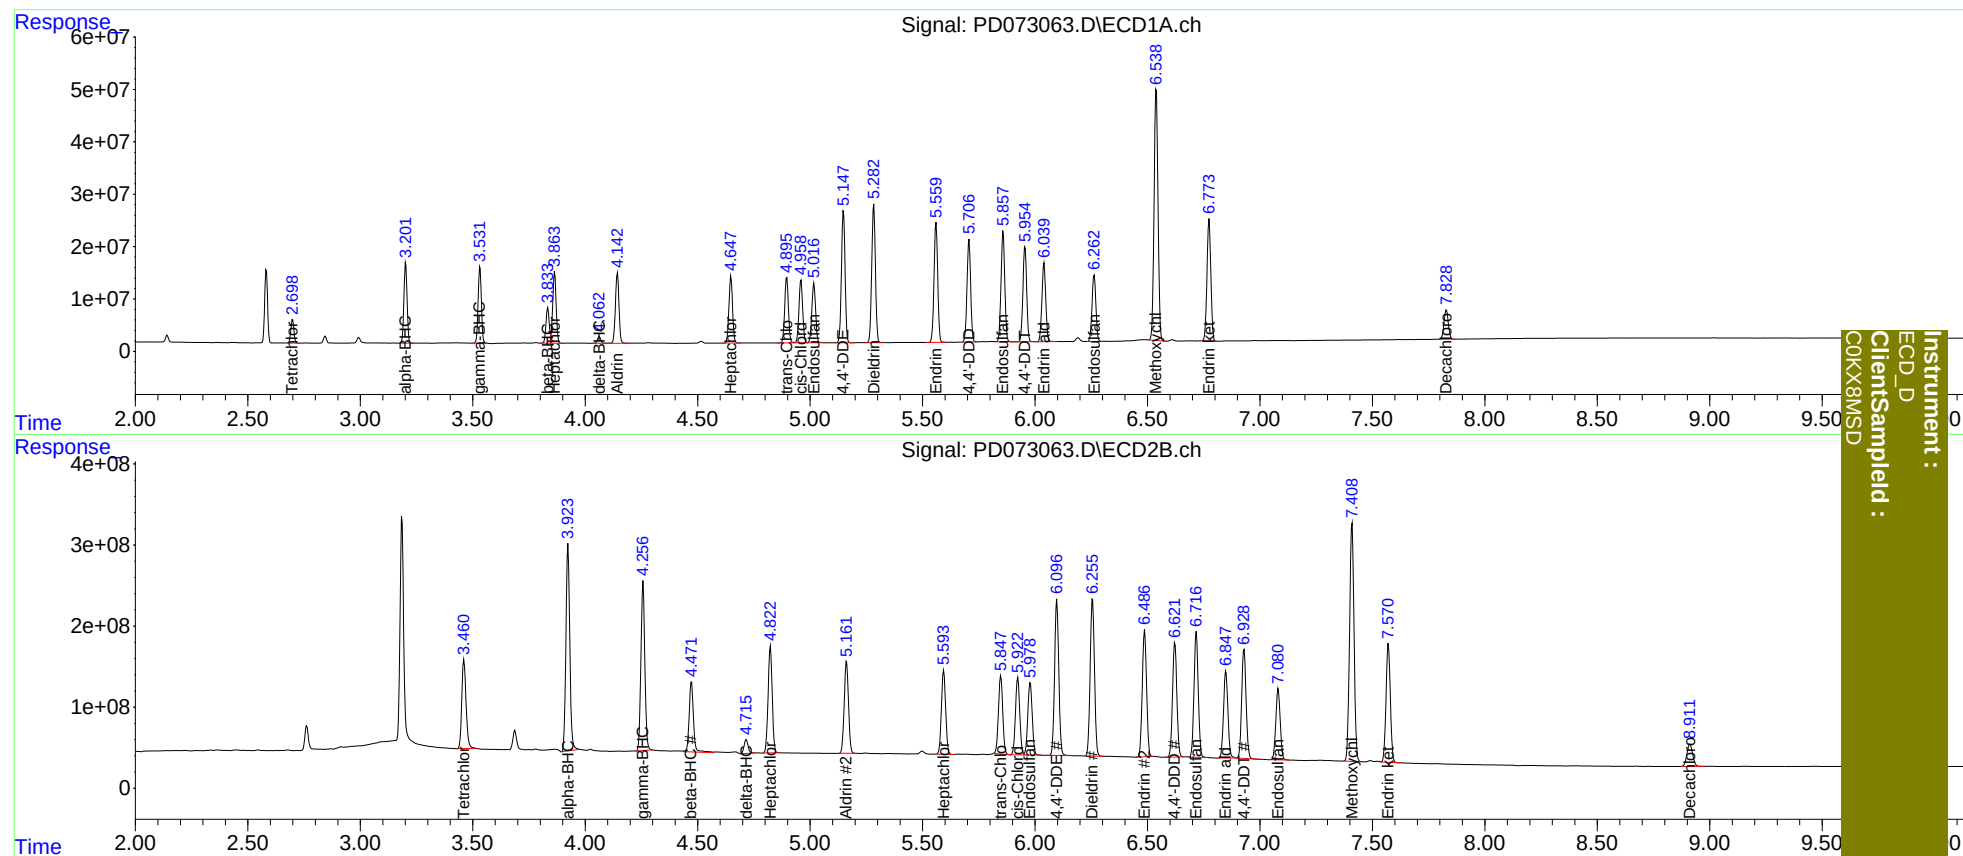

Instrument :
ECD_D
Client Sampled :
C0KX8MSD