

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD111822\  
 Data File : PD073068.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 17 Nov 2022 15:00  
 Operator : AR\AJ  
 Sample : N5574-02MS  
 Misc :  
 ALS Vial : 20 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 B0AA0MS

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 18 05:12:18 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD111722CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Nov 17 06:19:59 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm


|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml   |
|-----------------------------|-----------------|-------|-------|----------|----------|---------|---------|
| -----                       |                 |       |       |          |          |         |         |
| System Monitoring Compounds |                 |       |       |          |          |         |         |
| 1)                          | SA Tetrachlo... | 2.699 | 3.462 | 45600537 | 1505.7E6 | 19.016  | 23.049  |
| 2)                          | SA Decachlor... | 7.828 | 8.912 | 77036393 | 495.0E6  | 33.760  | 33.451  |
| Target Compounds            |                 |       |       |          |          |         |         |
| 2)                          | A alpha-BHC     | 3.202 | 3.924 | 161.7E6  | 3260.8E6 | 44.178  | 37.392  |
| 3)                          | MA gamma-BHC... | 3.532 | 4.258 | 160.6E6  | 2712.0E6 | 48.385  | 39.970  |
| 4)                          | MA Heptachlor   | 3.864 | 4.824 | 161.4E6  | 1862.3E6 | 48.325  | 40.554  |
| 5)                          | MB Aldrin       | 4.143 | 5.162 | 159.6E6  | 1612.7E6 | 47.371  | 40.156  |
| 6)                          | B beta-BHC      | 3.834 | 4.473 | 74462035 | 1228.7E6 | 46.378  | 45.988  |
| 7)                          | B delta-BHC     | 4.063 | 4.716 | 12194436 | 225.5E6  | 3.355   | 4.145   |
| 8)                          | B Heptachlo...  | 4.648 | 5.594 | 155.2E6  | 1490.5E6 | 49.954  | 44.096  |
| 9)                          | A Endosulfan I  | 5.017 | 5.979 | 142.0E6  | 1320.7E6 | 50.231  | 45.401  |
| 10)                         | B trans-Chl...  | 4.897 | 5.848 | 150.4E6  | 1362.2E6 | 48.806  | 43.121  |
| 11)                         | B cis-Chlor...  | 4.960 | 5.923 | 145.8E6  | 1338.8E6 | 46.560  | 42.172  |
| 12)                         | B 4,4'-DDE      | 5.148 | 6.097 | 295.7E6  | 2596.1E6 | 98.844  | 86.470  |
| 13)                         | MA Dieldrin     | 5.283 | 6.256 | 325.3E6  | 2833.8E6 | 106.195 | 94.012  |
| 14)                         | MA Endrin       | 5.560 | 6.487 | 286.2E6  | 2252.2E6 | 105.578 | 91.305  |
| 15)                         | B Endosulfa...  | 5.858 | 6.717 | 271.4E6  | 2235.6E6 | 100.795 | 92.541  |
| 16)                         | A 4,4'-DDD      | 5.707 | 6.622 | 236.6E6  | 2010.7E6 | 98.195  | 87.735  |
| 17)                         | MA 4,4'-DDT     | 5.955 | 6.930 | 232.1E6  | 1984.5E6 | 103.756 | 92.401  |
| 18)                         | B Endrin al...  | 6.040 | 6.848 | 197.4E6  | 1612.6E6 | 91.418  | 85.121  |
| 19)                         | B Endosulfa...  | 6.263 | 7.081 | 163.6E6  | 1297.4E6 | 65.204  | 62.391  |
| 20)                         | A Methoxychlor  | 6.539 | 7.409 | 644.7E6  | 4452.9E6 | 514.761 | 477.248 |
| 21)                         | B Endrin ke...  | 6.773 | 7.571 | 304.7E6  | 2149.9E6 | 104.392 | 96.289  |
| -----                       |                 |       |       |          |          |         |         |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD111822\  
Data File : PD073068.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 17 Nov 2022 15:00  
Operator : AR\AJ  
Sample : N5574-02MS  
Misc :  
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 18 05:12:18 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD111722CLP.M  
Quant Title : GC Extractables  
QLast Update : Thu Nov 17 06:19:59 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

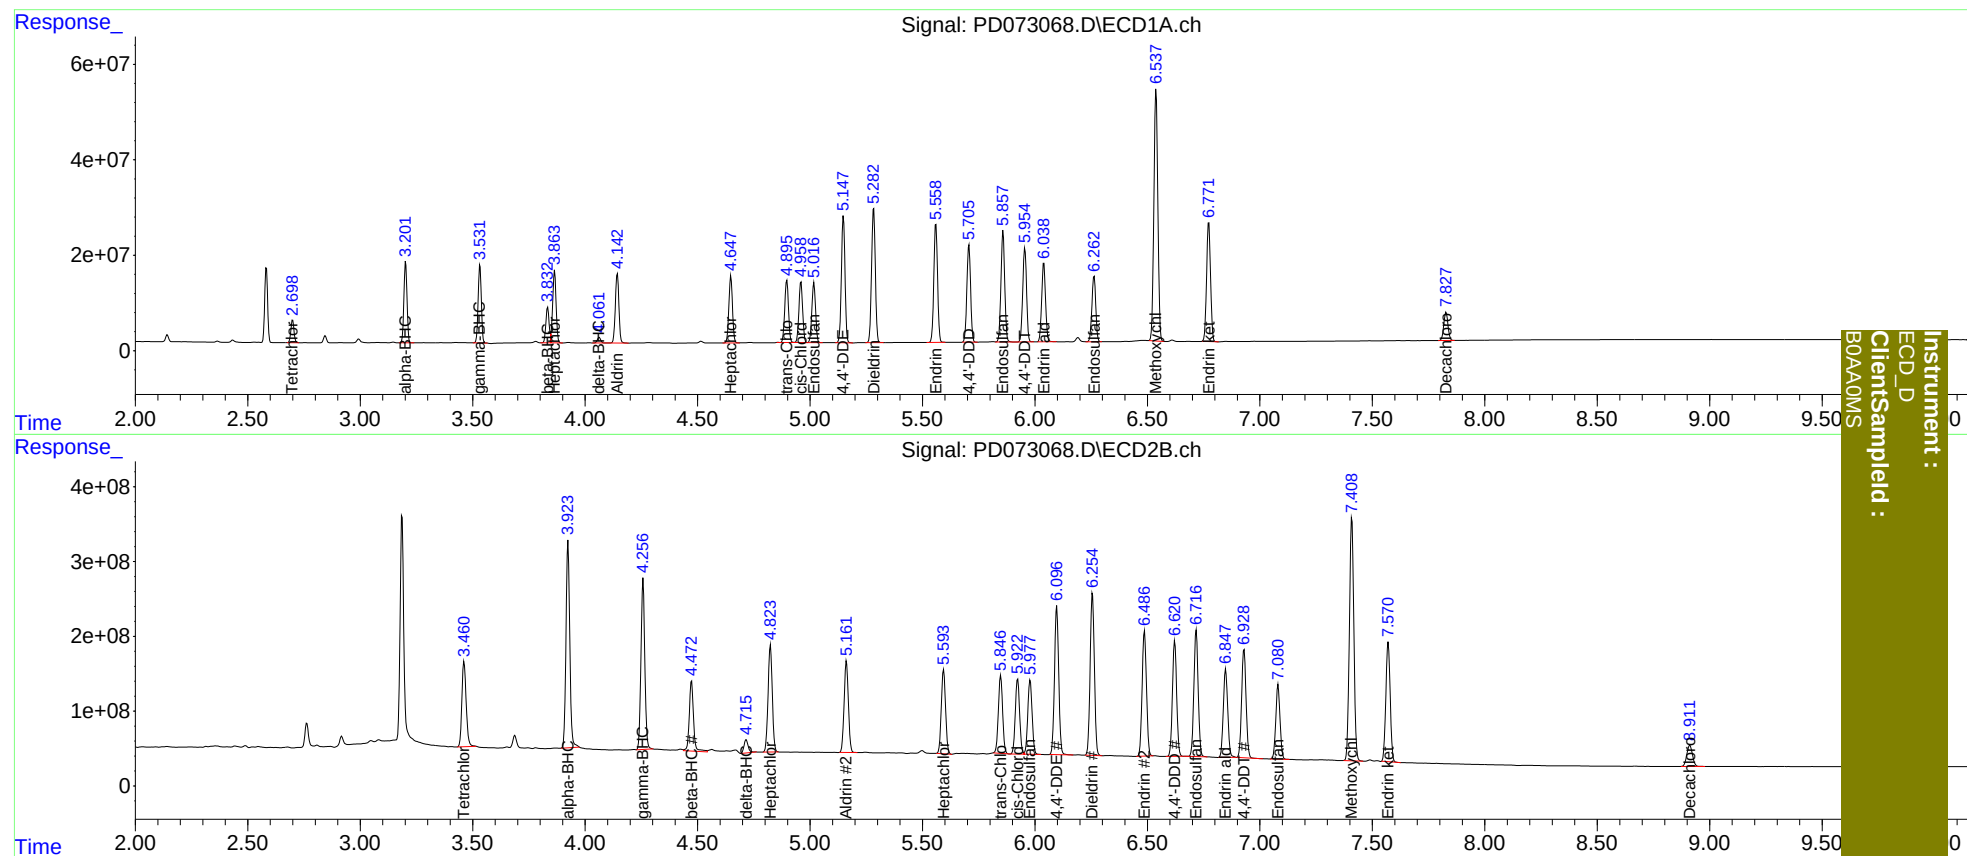

Instrument :  
ECD\_D  
ClientSampled :  
BOA/OMS