

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111822\
 Data File : PD073080.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2022 17:50
 Operator : AR\AJ
 Sample : PB149087BS
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS087

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/21/2022
 Supervised By : Ankita Jodhani 11/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 05:15:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.698	3.459	45525790	1173.2E6	18.985	17.959
27)	SA Decachlor...	7.827	8.911	87102503	567.0E6	38.171	38.314
Target Compounds							
2)	A alpha-BHC	3.201	3.923	16325725	423.9E6	4.461	4.861
3)	MA gamma-BHC...	3.531	4.257	15610652	357.0E6	4.704	5.261
4)	MA Heptachlor	3.863	4.823	15451704	234.1E6	4.625	5.098
5)	MB Aldrin	4.143	5.162	16176326	207.0E6	4.800	5.153
6)	B beta-BHC	3.833	4.471	7832227	131.2E6	4.878	4.910m
7)	B delta-BHC	4.062	4.716	15564539	270.9E6	4.282	4.978
8)	B Heptachlo...	4.647	5.593	14899592	174.3E6	4.795	5.157m
9)	A Endosulfan I	5.016	5.978	13737510	148.8E6	4.861	5.115
10)	B trans-Chl...	4.895	5.848	14971681	158.0E6	4.858	5.000
11)	B cis-Chlor...	4.959	5.923	14975422	157.8E6	4.783	4.970
12)	B 4,4'-DDE	5.147	6.097	26329188	289.8E6	8.801	9.652
13)	MA Dieldrin	5.282	6.255	28349249	308.1E6	9.254	10.220
14)	MA Endrin	5.559	6.487	25269916	237.6E6	9.321	9.633
15)	B Endosulfa...	5.857	6.717	25401067	247.5E6	9.432	10.244
16)	A 4,4'-DDD	5.706	6.621	22245705	233.9E6	9.233	10.206
17)	MA 4,4'-DDT	5.955	6.929	19676721	207.2E6	8.796	9.646
18)	B Endrin al...	6.039	6.848	21084552	190.5E6	9.762	10.054
19)	B Endosulfa...	6.262	7.080	23476592	205.0E6	9.357	9.857
20)	A Methoxychlor	6.538	7.408	61278384	484.0E6	48.926	51.878
21)	B Endrin ke...	6.773	7.570	29080802	233.2E6	9.962	10.444

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111822\
Data File : PD073080.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2022 17:50
Operator : AR\AJ
Sample : PB149087BS
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 05:15:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

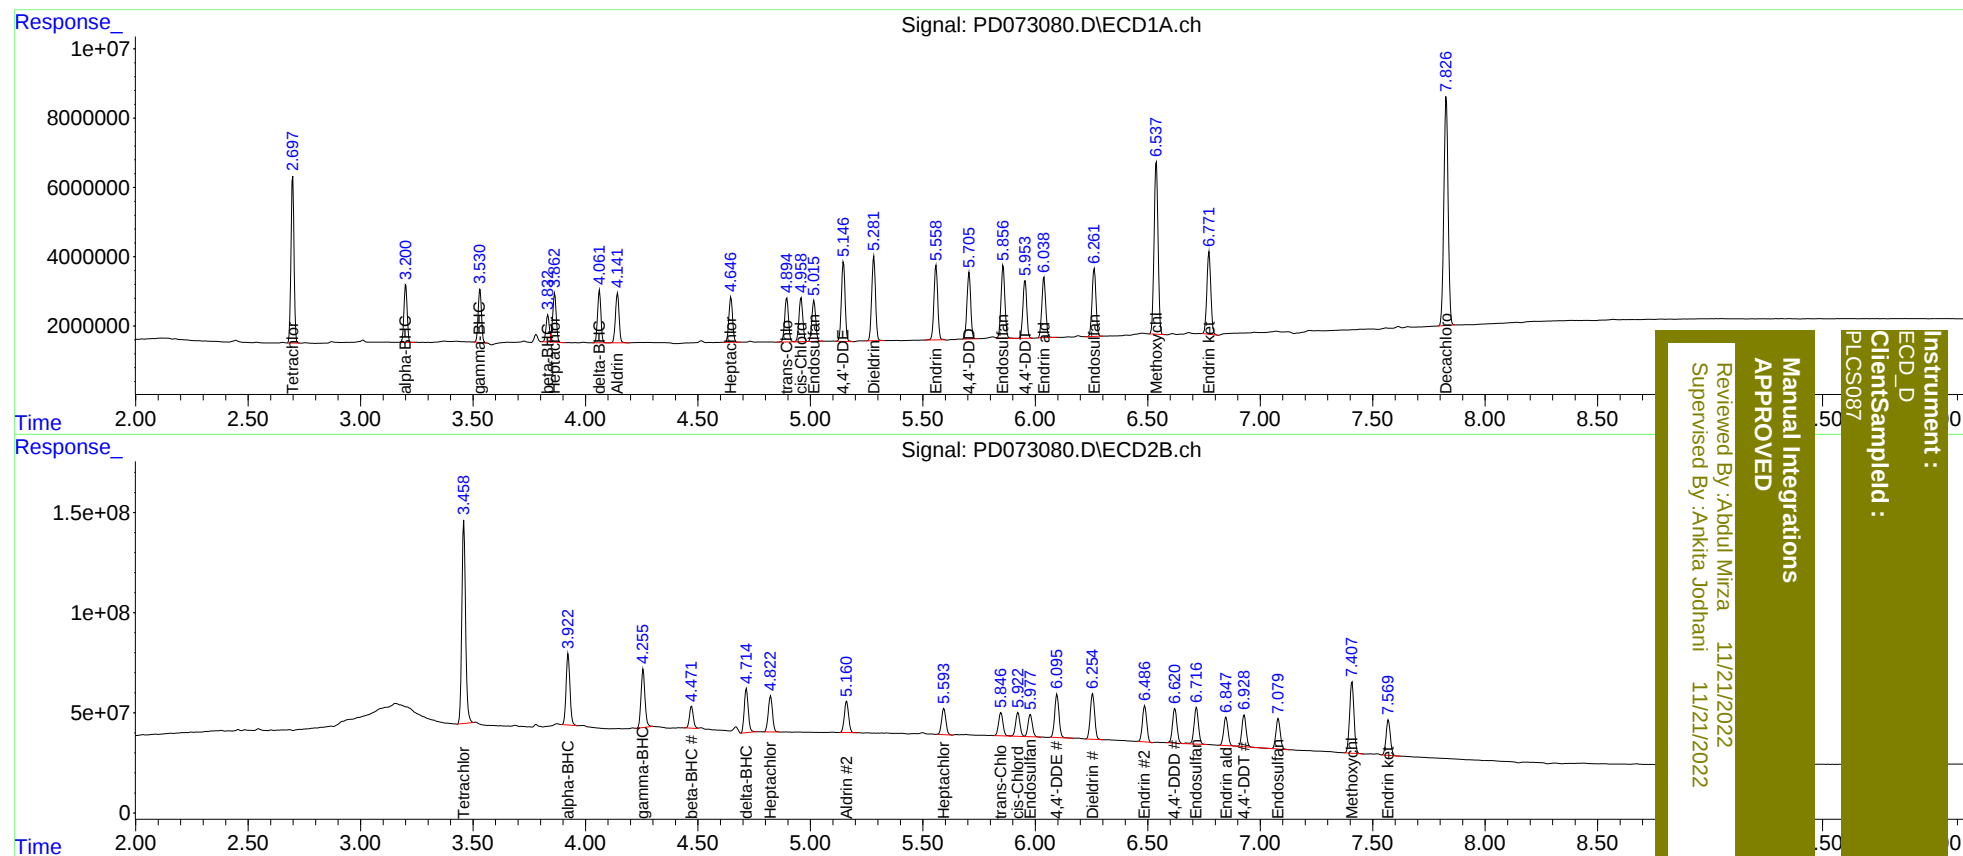

Instrument :
ECD_D
ClientSampled :
PLCS087

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 11/21/2022
Supervised By: Ankita Jodhani 11/21/2022