

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111919\
 Data File : PD056096.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2019 15:59
 Operator : SG\AJ
 Sample : K5820-10
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0B03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 00:31:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.292	3.963	21426368	29529488	28.463	28.178
27) SA Decachlor...	7.969	9.001	28291100	34131674	34.708	30.057
Target Compounds						
10) B trans-Chl...	0.000	6.045	0	5599986	N.D.	3.926
21) B Endrin ke...	0.000	7.736f	0	2273978	N.D.	1.724


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111919\
Data File : PD056096.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2019 15:59
Operator : SG\AJ
Sample : K5820-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0B03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 00:31:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

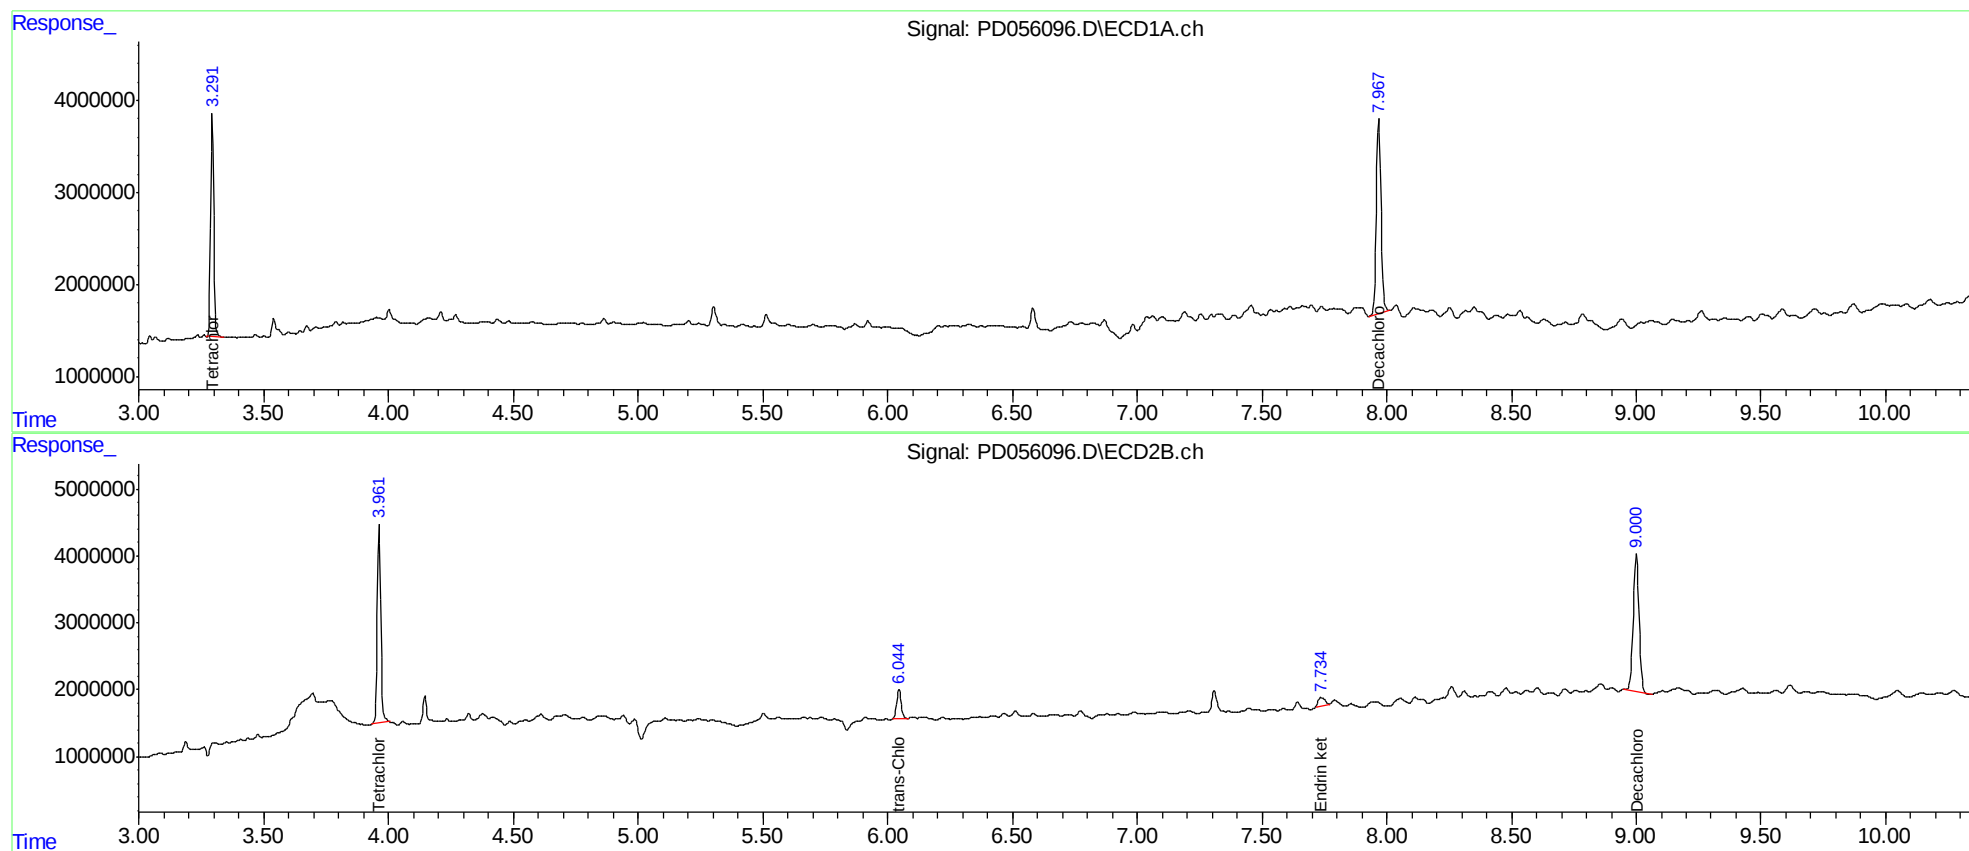


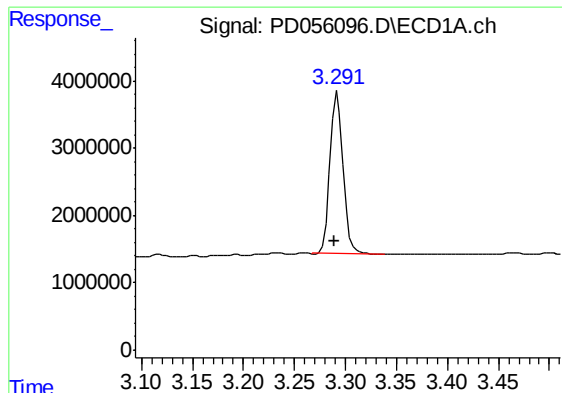

#1 Tetrachloro-m-xylene


R.T.: 3.292 min
Delta R.T.: 0.003 min
Response: 21426368
Conc: 28.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0B03

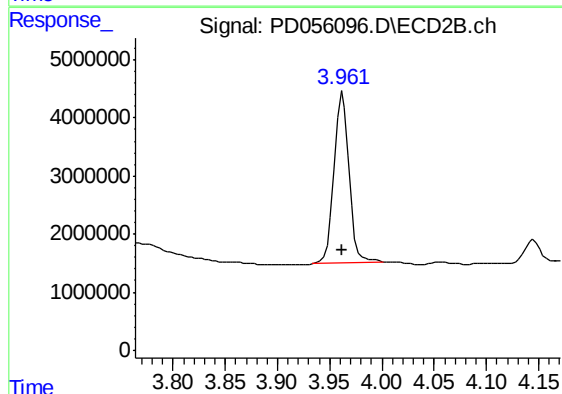


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 29529488
Conc: 28.18 ng/ml

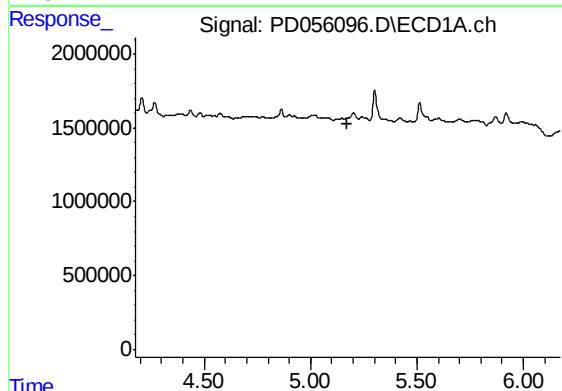


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

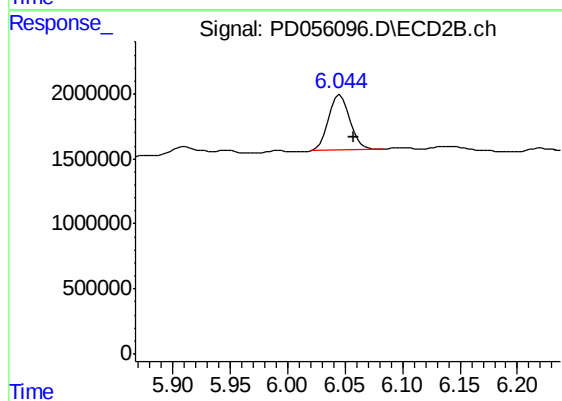

#10 trans-Chlordane


R.T.: 6.045 min
Delta R.T.: -0.013 min
Response: 5599986
Conc: 3.93 ng/ml

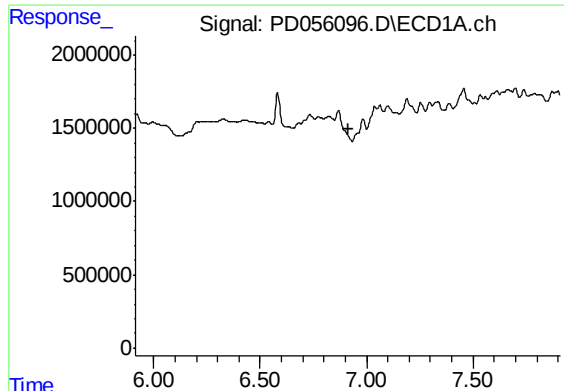

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.913 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0B03

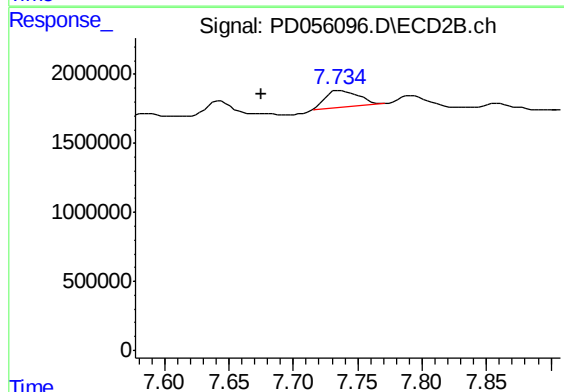


#21 Endrin ketone

R.T.: 7.736 min
Delta R.T.: 0.061 min
Response: 2273978
Conc: 1.72 ng/ml

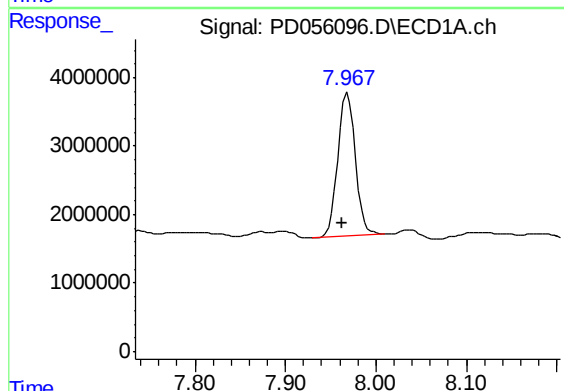

#27 Decachlorobiphenyl

R.T.: 7.969 min
Delta R.T.: 0.006 min
Response: 28291100
Conc: 34.71 ng/ml

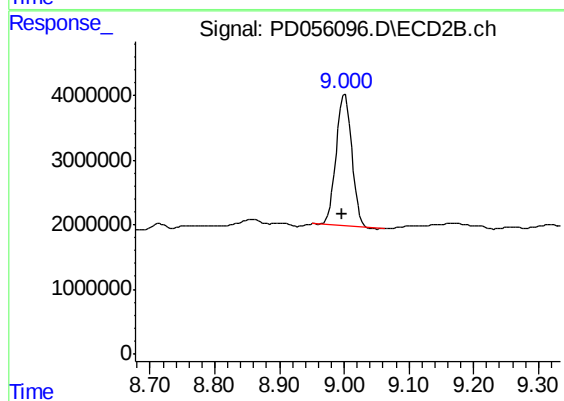

#27 Decachlorobiphenyl

R.T.: 9.001 min
Delta R.T.: 0.004 min
Response: 34131674
Conc: 30.06 ng/ml