

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111920\
 Data File : PD060124.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2020 09:58
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 03:42:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 04:05:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
8) B	Heptachlo...	5.175f	5.895	688567	29474201	0.652 8.949 #
14) MA	Endrin	0.000	6.804f	0	26487470	N.D. 9.460
16) A	4,4'-DDD	0.000	6.804f	0	26487470	N.D. 9.873
20) A	Methoxychlor	0.000	7.551f	0	1519449	N.D. 1.081


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111920\
Data File : PD060124.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2020 09:58
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 03:42:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

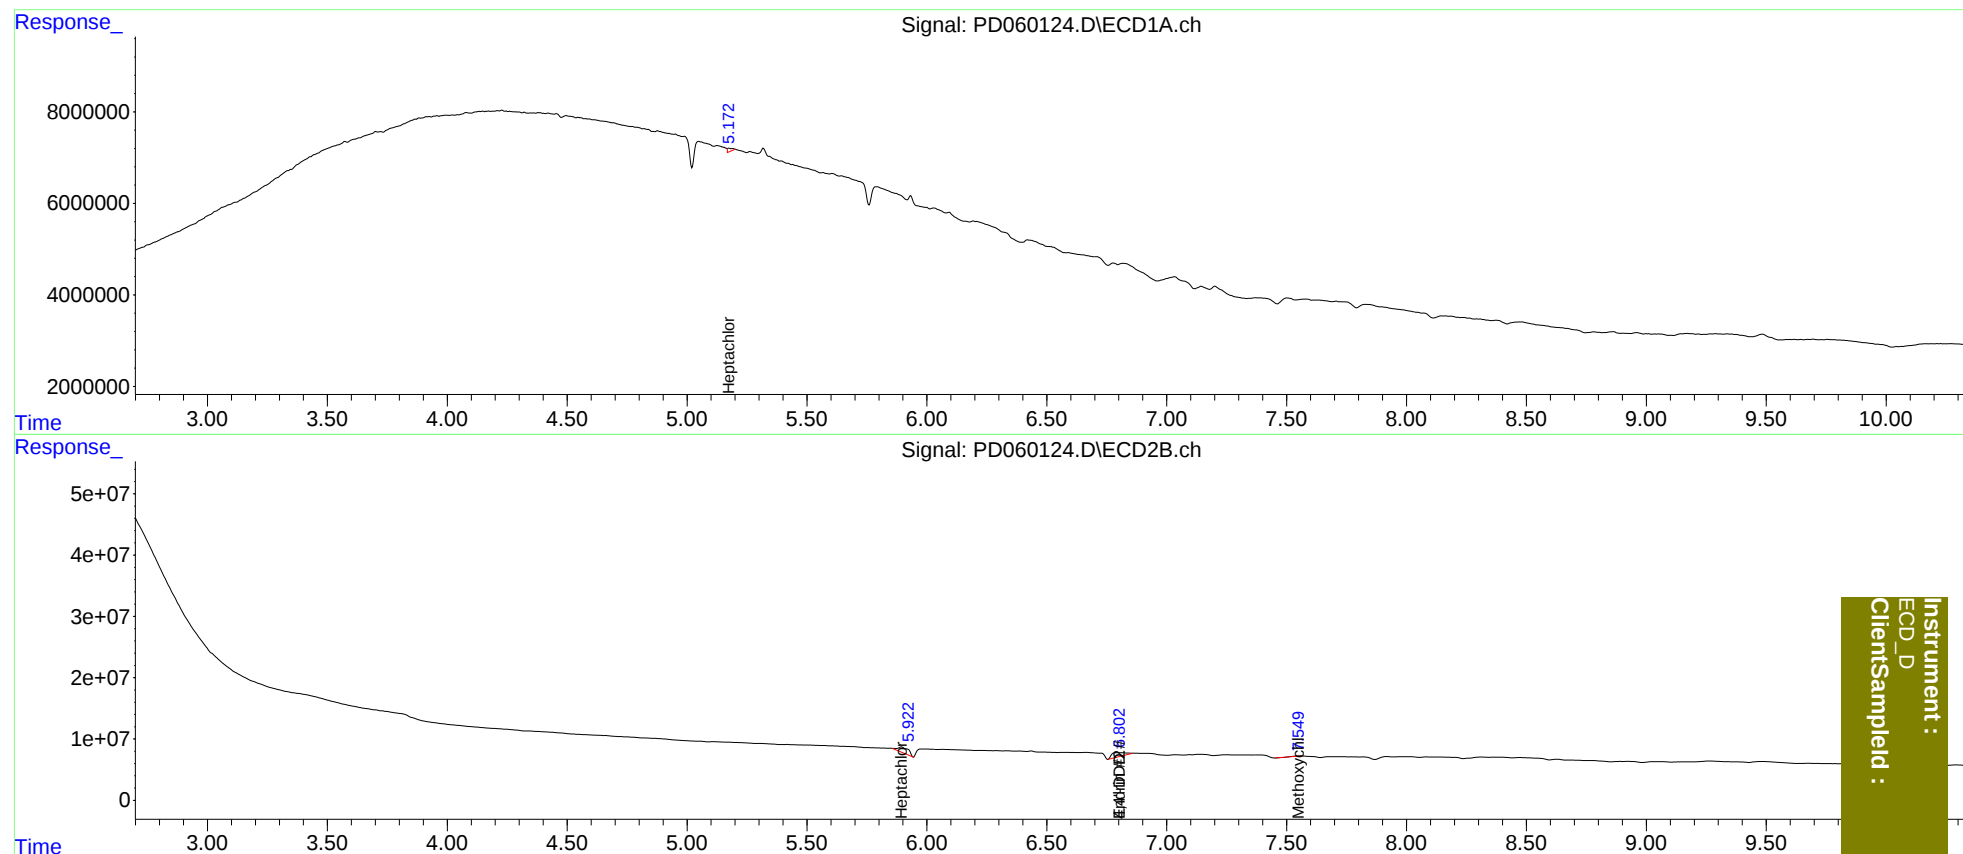


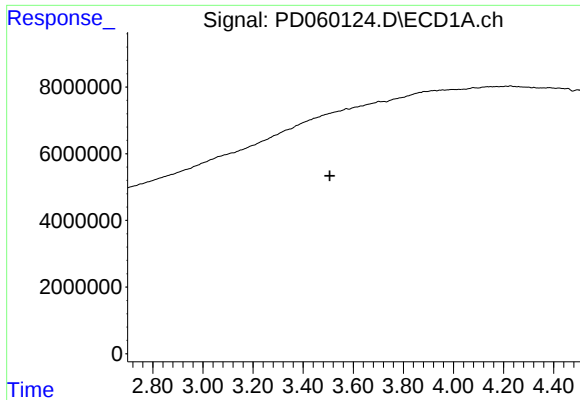

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.506 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

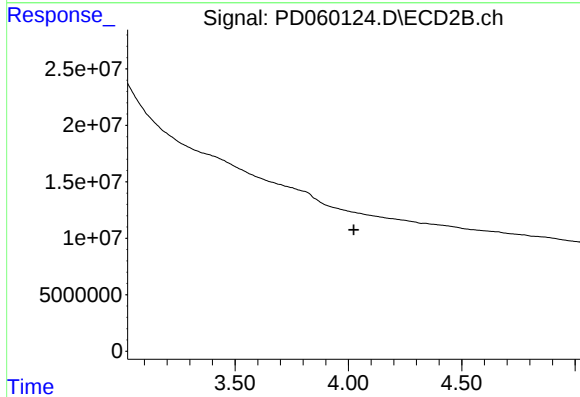


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.024 min
Response: 0
Conc: N.D.

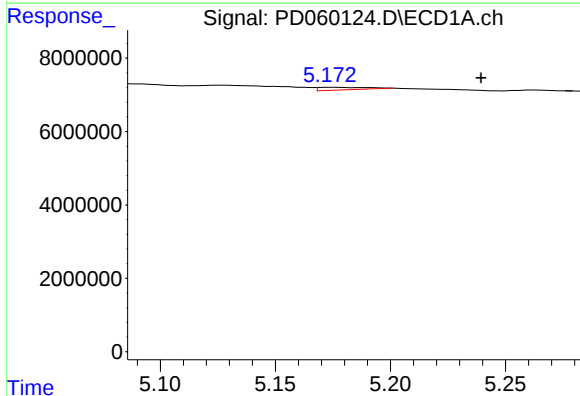


#8 Heptachlor epoxide

R.T.: 5.175 min
Delta R.T.: -0.065 min
Response: 688567
Conc: 0.65 ng/ml

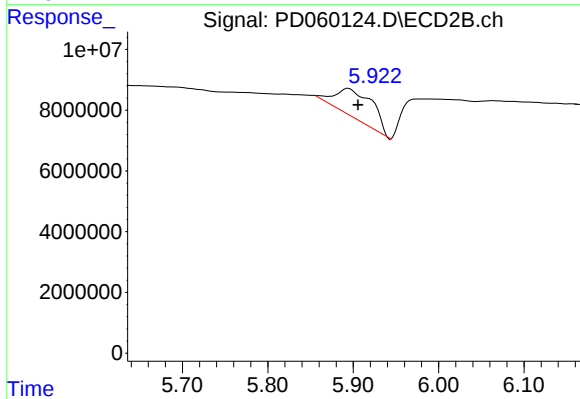

#8 Heptachlor epoxide


R.T.: 5.895 min
Delta R.T.: -0.011 min
Response: 29474201
Conc: 8.95 ng/ml

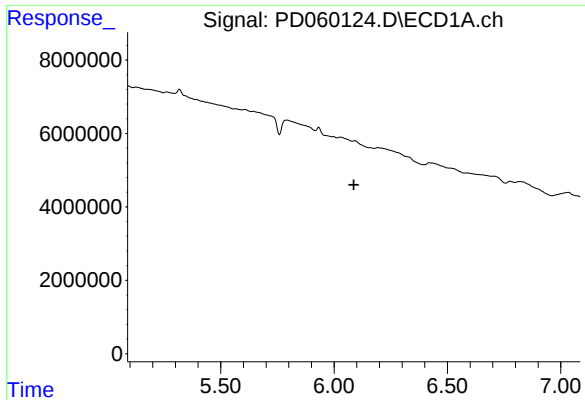

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.087 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

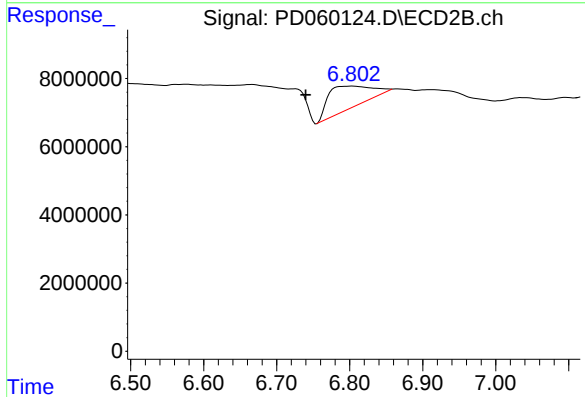


#14 Endrin

R.T.: 6.804 min
Delta R.T.: 0.064 min
Response: 26487470
Conc: 9.46 ng/ml

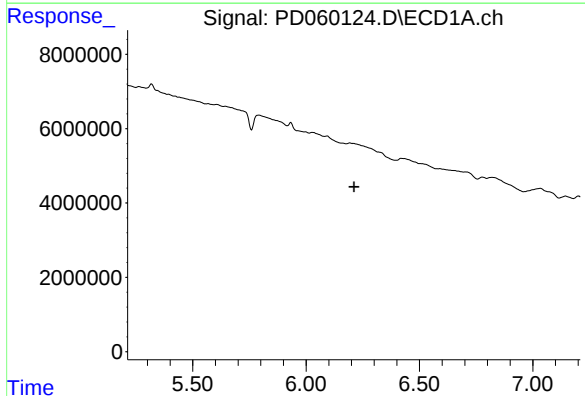


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.212 min
Response: 0
Conc: N.D.

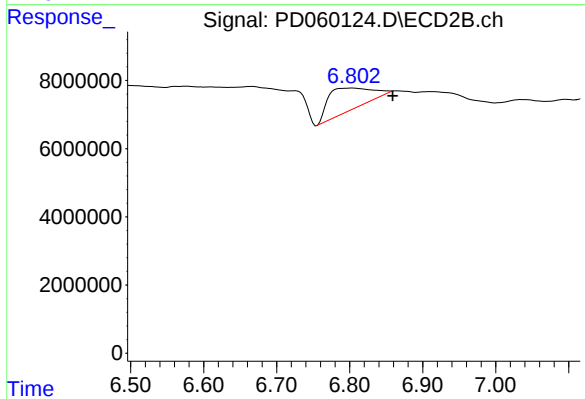

#16 4,4'-DDD


R.T.: 6.804 min
Delta R.T.: -0.055 min
Response: 26487470
Conc: 9.87 ng/ml

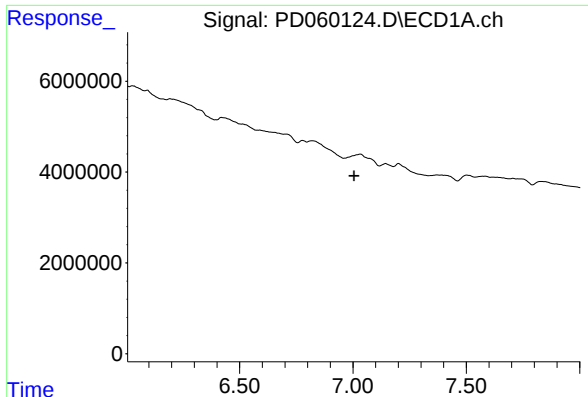

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.005 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

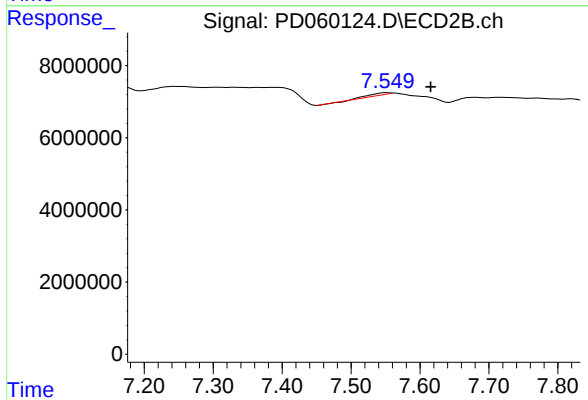


#20 Methoxychlor

R.T.: 7.551 min
Delta R.T.: -0.065 min
Response: 1519449
Conc: 1.08 ng/ml

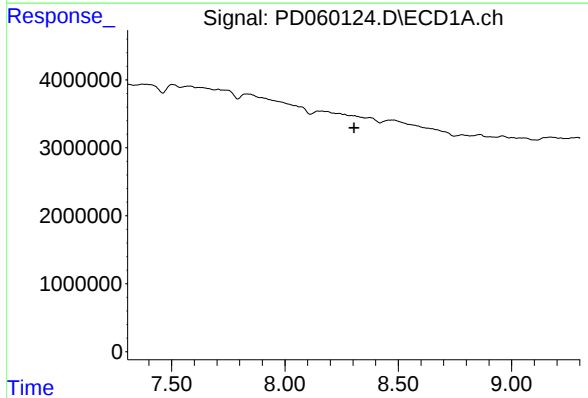

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.305 min
Response: 0
Conc: N.D.

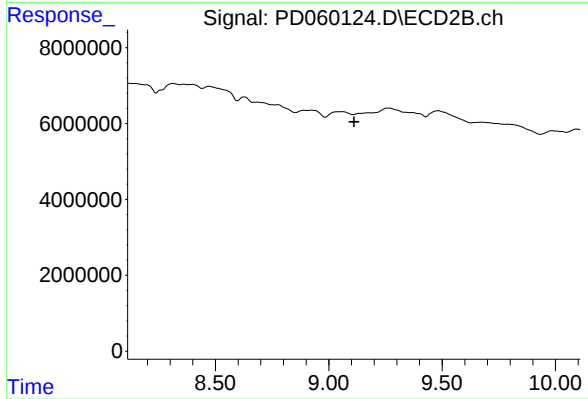

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.112 min
Response: 0
Conc: N.D.