

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111921\
 Data File : PD067011.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2021 10:03
 Operator : AR\AJ
 Sample : PB140615BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS615

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/22/2021
 Supervised By :Ankita Jodhani 11/22/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 03:38:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 27 16:50:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.967	37236532	191.5E6	19.263	22.114
27)	SA Decachlor...	8.163	9.026	39088679	211.7E6	33.361	40.583
Target Compounds							
2)	A alpha-BHC	3.874	4.360	10468404	47671852	3.576	4.360
3)	MA gamma-BHC...	4.156	4.645	11314938	48243133	4.087	4.774
4)	MA Heptachlor	4.449	5.145	12114902	49123760	4.259	5.012
5)	MB Aldrin	4.694	5.448	12531454	46465041	4.352	4.931
6)	B beta-BHC	4.404	4.822	5732668	26376014	4.564	5.353
7)	B delta-BHC	4.605	5.038	911746	6984975	0.344	0.706 #
8)	B Heptachlo...	5.135	5.837	11916768	42077518	4.688	5.597
9)	A Endosulfan I	5.471	6.195	10903409	42055925	4.757	5.375
10)	B trans-Chl...	5.358	6.072	12078975	44568448	4.673	5.176
11)	B cis-Chlor...	5.417	6.143	11859325	44687915	4.655	5.208
12)	B 4,4'-DDE	5.580	6.303	21590014	81301046	9.453	10.677
13)	MA Dieldrin	5.713	6.453	22419774	84381280	8.984	10.577
14)	MA Endrin	5.969	6.672	17540365	60838955	8.290	8.965
15)	B Endosulfa...	6.241	6.887	18899043	74279307	9.102m	10.358
16)	A 4,4'-DDD	6.095	6.798	16563274	67204337	9.151	10.410
17)	MA 4,4'-DDT	6.334	7.096	15132997	59587317	8.004	9.020
18)	B Endrin al...	6.410	7.012	16803536	65168894	11.534m	12.249
19)	B Endosulfa...	6.623	7.234	11990648	48591493	6.573	7.051
20)	A Methoxychlor	6.881	7.558	41074299	150.5E6	43.826	46.556
21)	B Endrin ke...	7.114	7.708	20187165	77329248	9.797	9.866

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111921\
Data File : PD067011.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2021 10:03
Operator : AR\AJ
Sample : PB140615BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 03:38:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 27 16:50:52 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

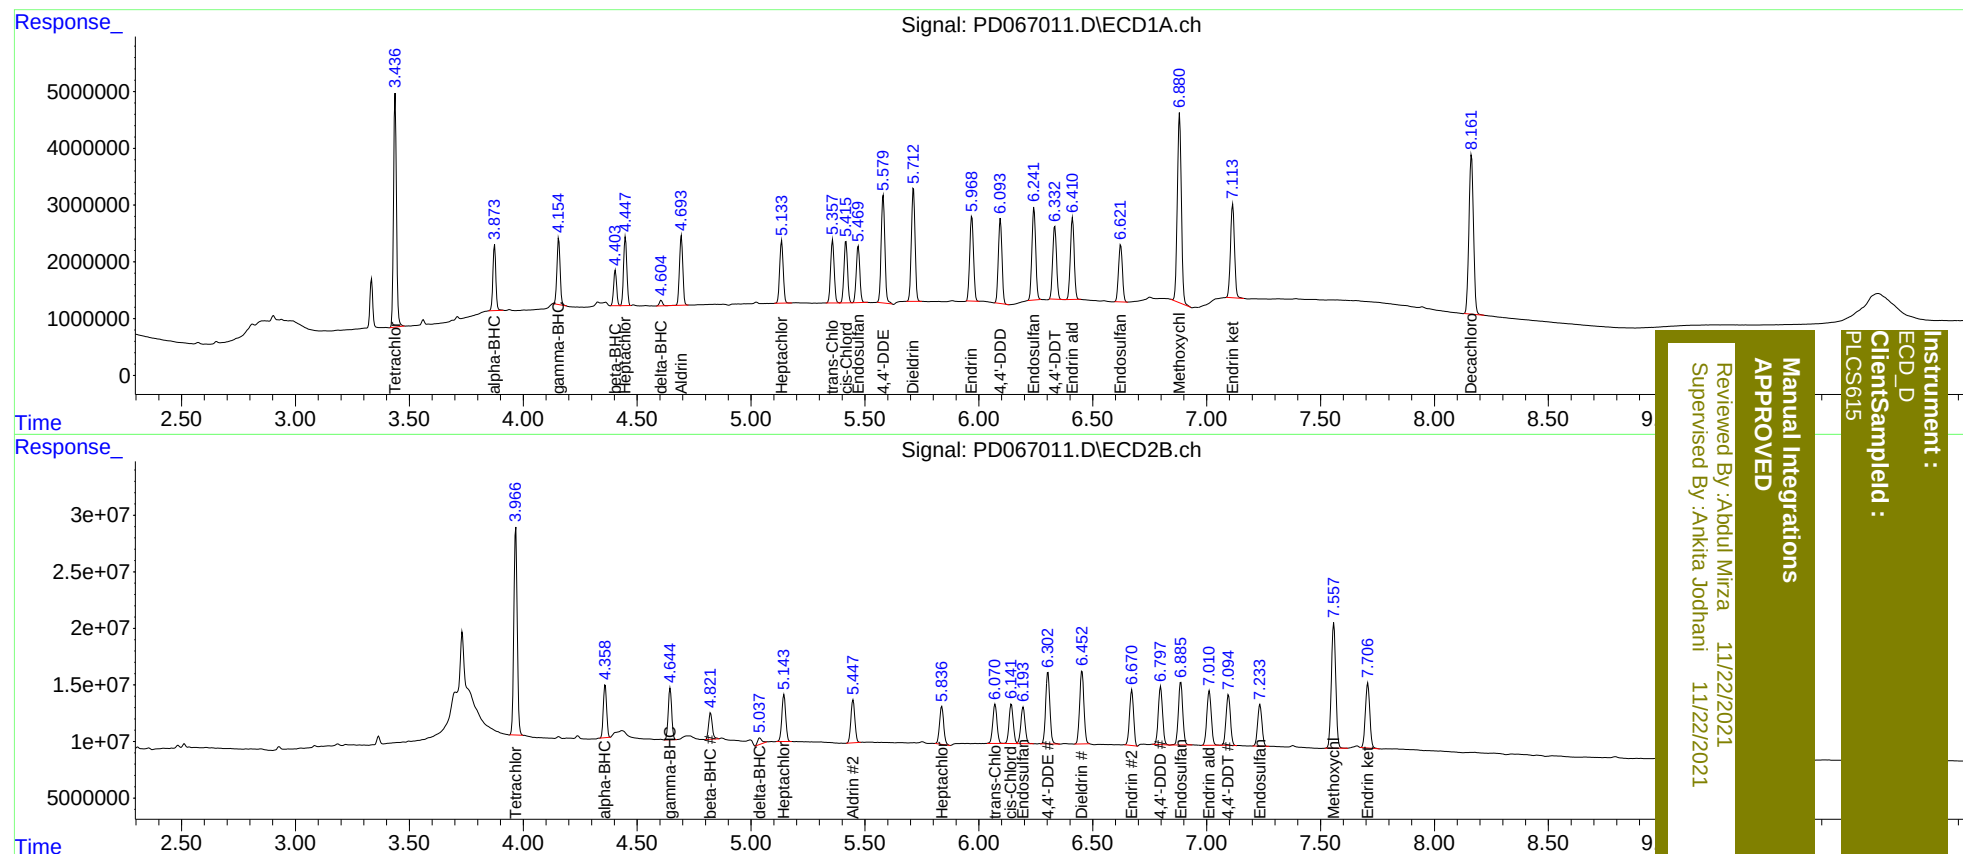

Instrument :
ECD_D
ClientSampled :
PLCS615

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 11/22/2021
Supervised By: Ankita Jodhani 11/22/2021