

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111922\
 Data File : PD073106.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2022 10:11
 Operator : AR\AJ
 Sample : PIBLK408
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 05:11:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.699	3.459	47535569	1356.1E6	19.823	20.760
27)	SA Decachlor...	7.828	8.910	80076593	539.7E6	35.092	36.470
Target Compounds							
2)	A alpha-BHC	0.000	3.933	0	18696396	N.D.	0.214
3)	MA gamma-BHC...	0.000	4.268	0	2170529	N.D.	<MDL
4)	MA Heptachlor	0.000	4.843	0	124961	N.D.	<MDL
5)	MB Aldrin	0.000	5.172	0	2226252	N.D.	<MDL
6)	B beta-BHC	0.000	4.477	0	9640571	N.D.	0.361
7)	B delta-BHC	0.000	4.731	0	4289519	N.D.	<MDL
8)	B Heptachlo...	0.000	5.592	0	54569730	N.D.	1.614
9)	A Endosulfan I	0.000	5.989	0	827709	N.D.	<MDL
10)	B trans-Chl...	0.000	5.850	0	573918	N.D.	<MDL
11)	B cis-Chlor...	0.000	5.946	0	504594	N.D.	<MDL
12)	B 4,4'-DDE	0.000	6.119	0	1975147	N.D.	<MDL
13)	MA Dieldrin	0.000	6.248	0	12279100	N.D.	0.407
14)	MA Endrin	5.556	0.000	40097	0	<MDL	N.D. #
15)	B Endosulfa...	5.855	0.000	173174	0	<MDL	N.D. #
16)	A 4,4'-DDD	5.659f	6.601	128317	817200	<MDL	<MDL #
17)	MA 4,4'-DDT	5.899f	6.960	37102	1544763	<MDL	<MDL #
19)	B Endosulfa...	6.265	0.000	87003	0	<MDL	N.D. #
20)	A Methoxychlor	6.469f	0.000	306761	0	0.245	N.D. #
22)	Toxaphene-1	0.000	5.776	0	2855998	N.D.	24.305
23)	Toxaphene-2	5.593	6.119	185213	1975147	11.845	9.217
24)	Toxaphene-3	5.899	6.960	37102	1544763	1.726	3.077 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111922\
Data File : PD073106.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2022 10:11
Operator : AR\AJ
Sample : PIBLK408
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 05:11:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

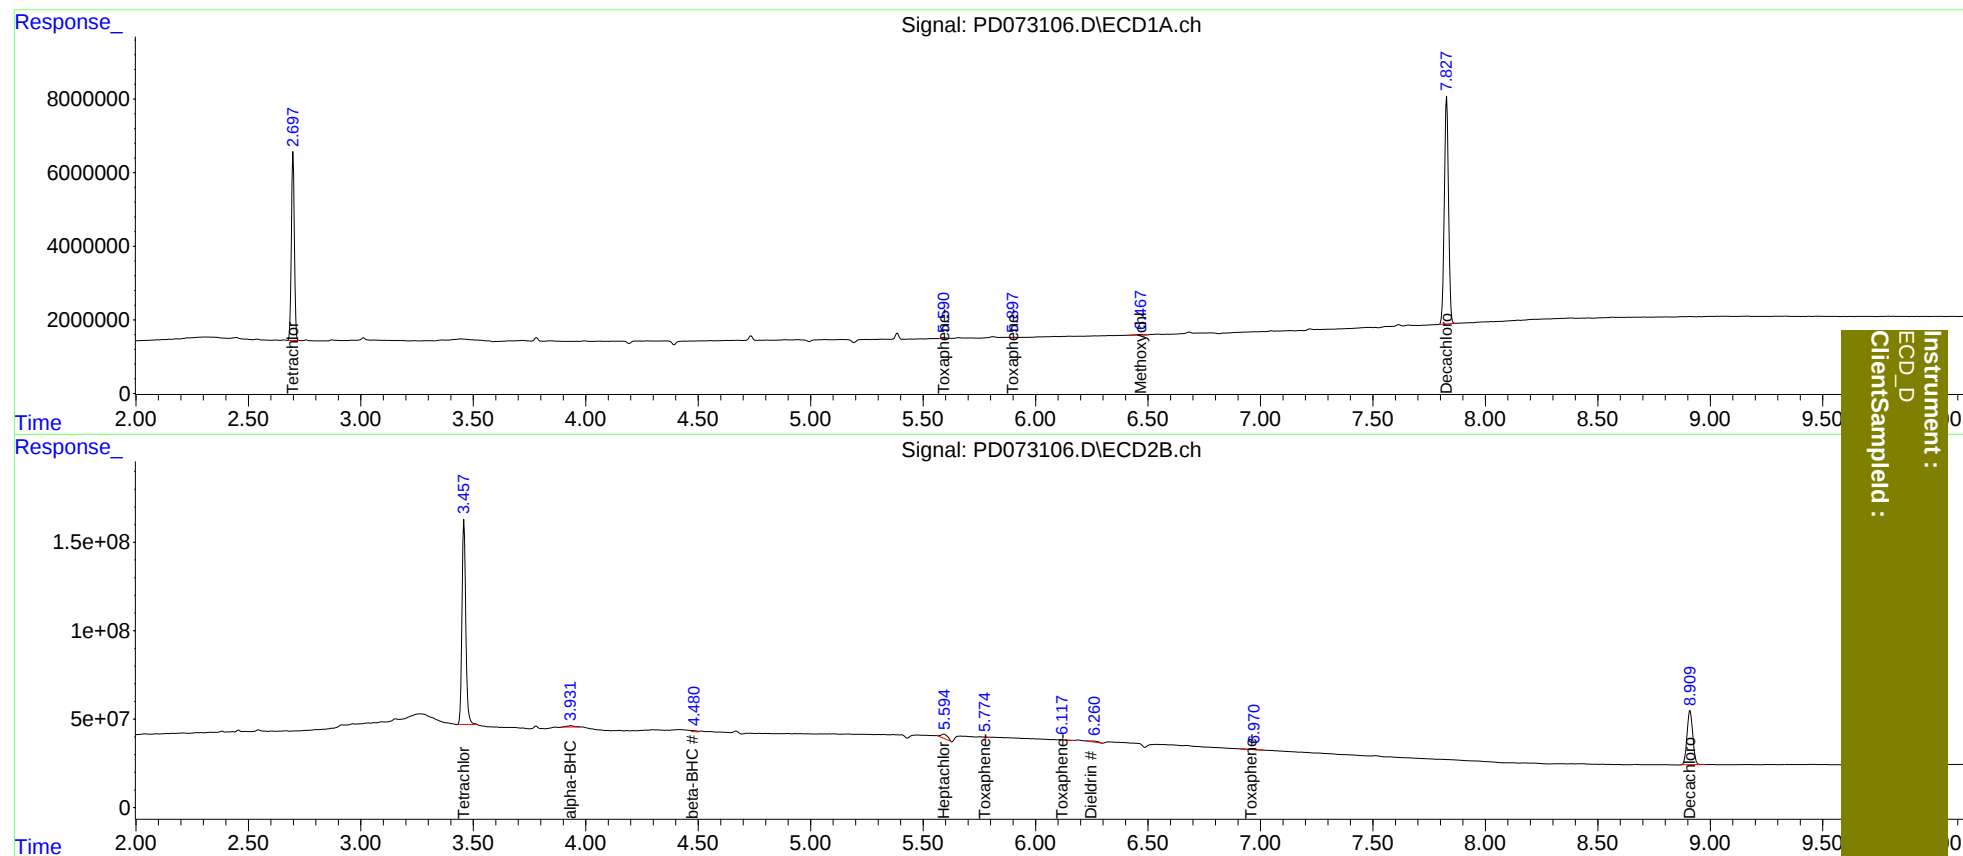


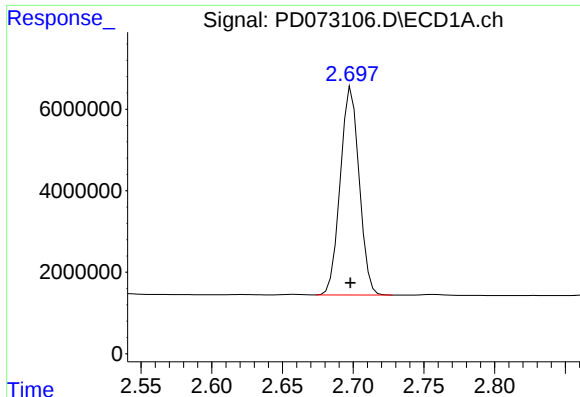

#1 Tetrachloro-m-xylene


R.T.: 2.699 min
Delta R.T.: 0.000 min
Response: 47535569
Conc: 19.82 ng/ml

Instrument :
ECD_D
ClientSampleId :

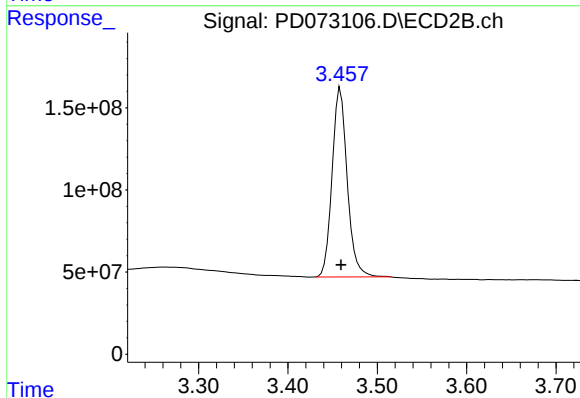


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 1356127404
Conc: 20.76 ng/ml

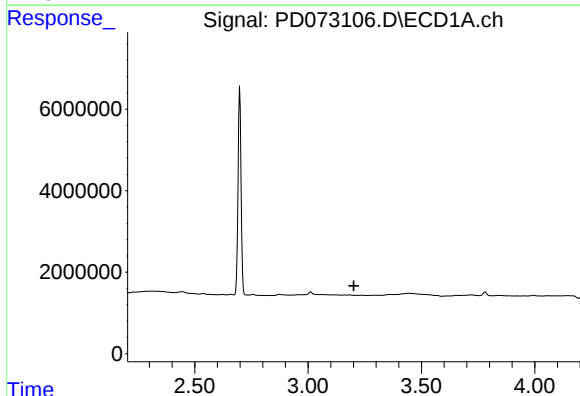


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.201 min
Response: 0
Conc: N.D.

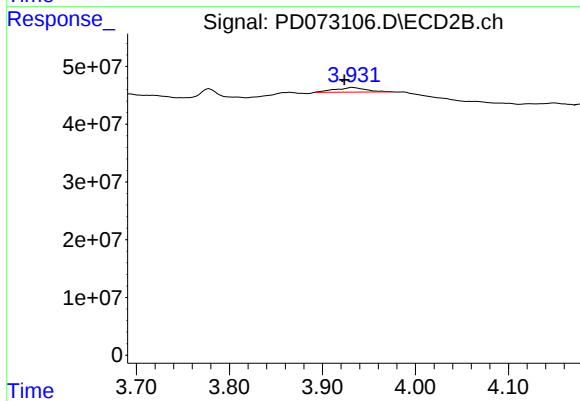

#2 alpha-BHC


R.T.: 3.933 min
Delta R.T.: 0.009 min
Response: 18696396
Conc: 0.21 ng/ml

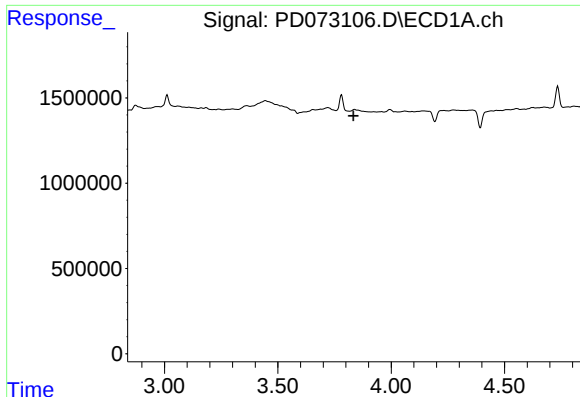

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 3.834 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

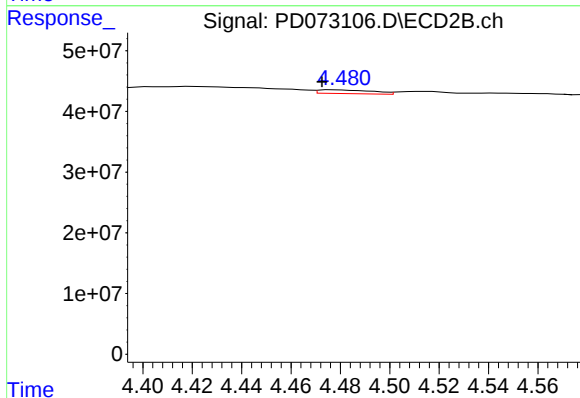


#6 beta-BHC

R.T.: 4.477 min
Delta R.T.: 0.004 min
Response: 9640571
Conc: 0.36 ng/ml

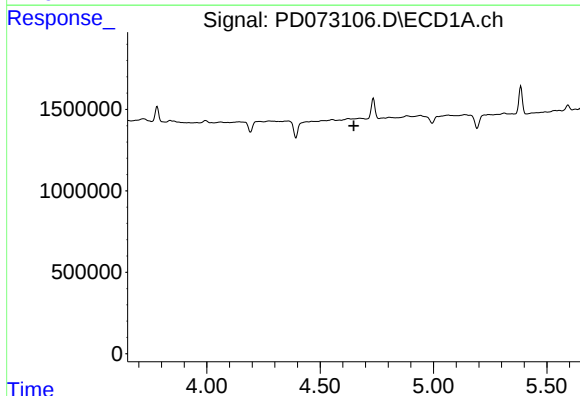


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.649 min
Response: 0
Conc: N.D.

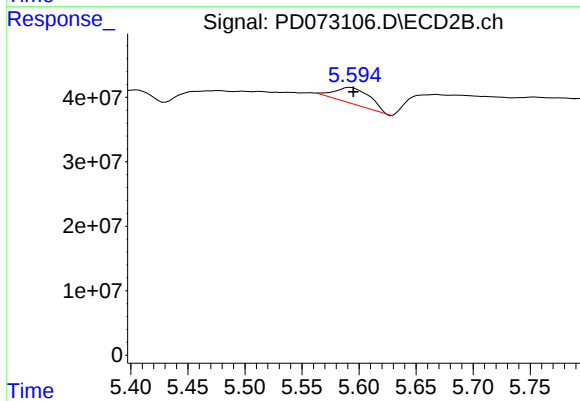

#8 Heptachlor epoxide


R.T.: 5.592 min
Delta R.T.: -0.002 min
Response: 54569730
Conc: 1.61 ng/ml

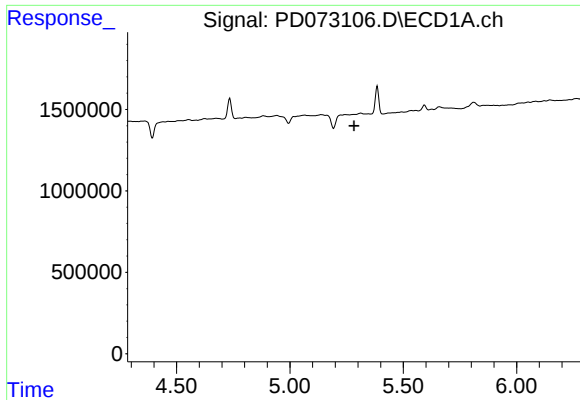

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

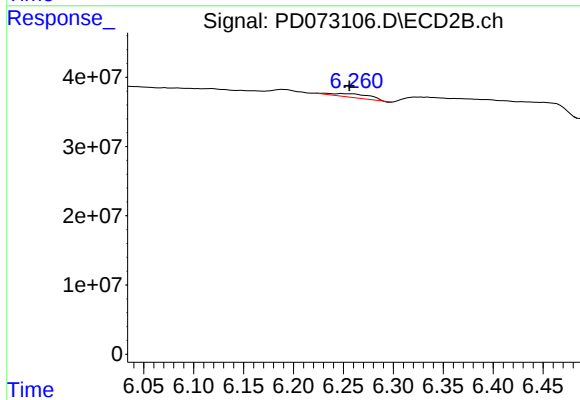


#13 Dieldrin

R.T.: 6.248 min
Delta R.T.: -0.008 min
Response: 12279100
Conc: 0.41 ng/ml

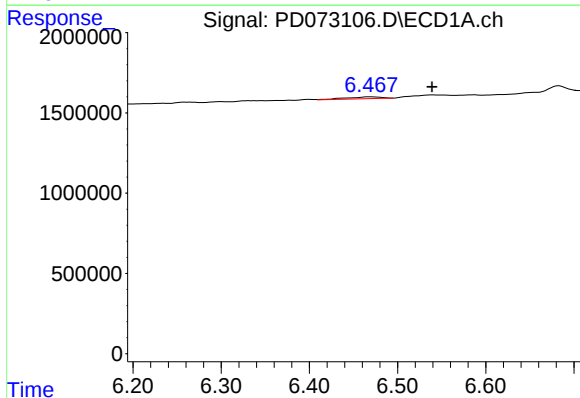


#20 Methoxychlor

R.T.: 6.469 min
Delta R.T.: -0.070 min
Response: 306761
Conc: 0.24 ng/ml

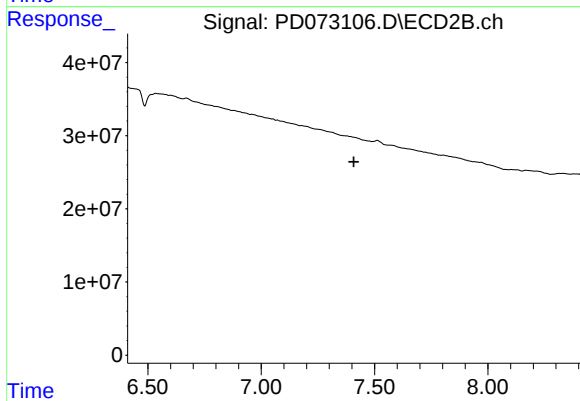

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.409 min
Response: 0
Conc: N.D.

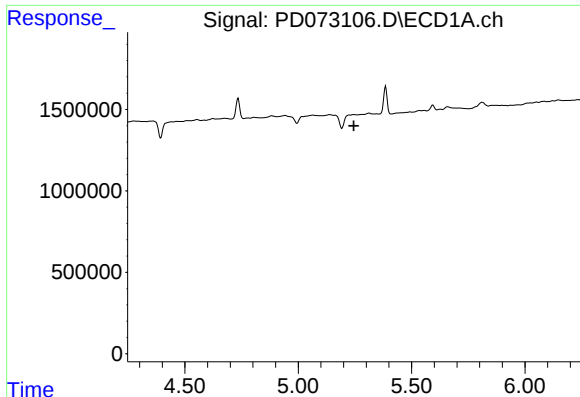

#22 Toxaphene-1


R.T.: 0.000 min
Exp R.T.: 5.246 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

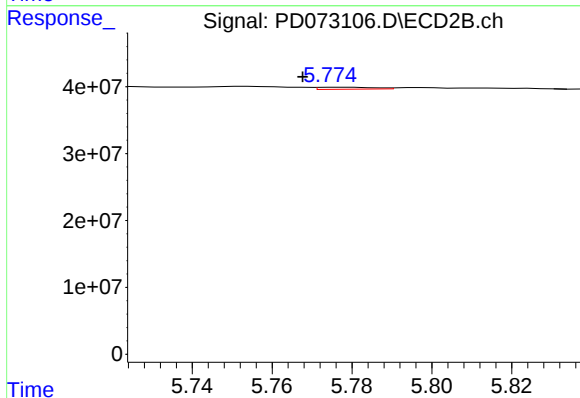


#22 Toxaphene-1

R.T.: 5.776 min
Delta R.T.: 0.009 min
Response: 2855998
Conc: 24.30 ng/ml

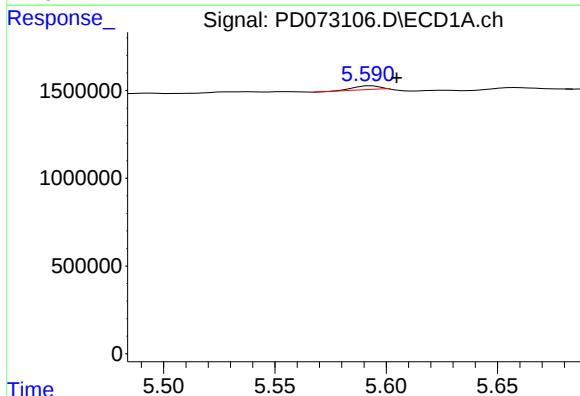


#23 Toxaphene-2

R.T.: 5.593 min
Delta R.T.: -0.011 min
Response: 185213
Conc: 11.84 ng/ml

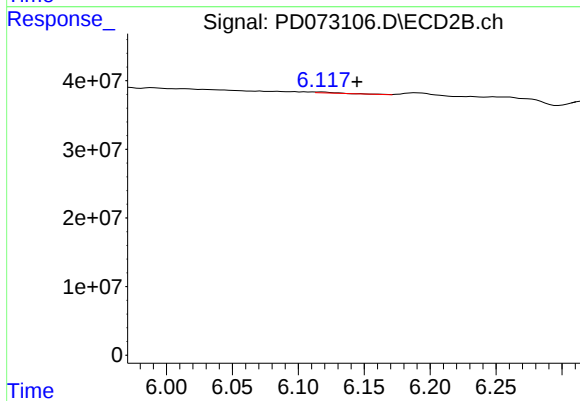

#23 Toxaphene-2


R.T.: 6.119 min
Delta R.T.: -0.026 min
Response: 1975147
Conc: 9.22 ng/ml

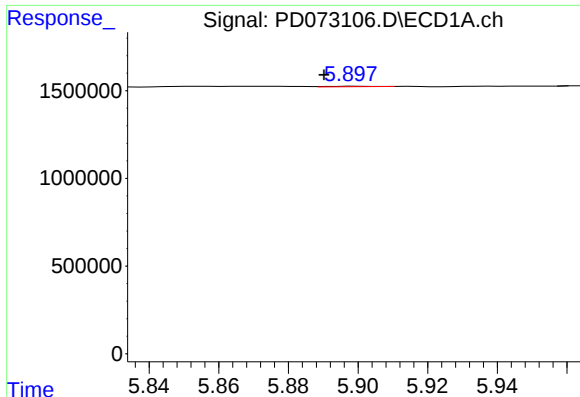

#24 Toxaphene-3


R.T.: 5.899 min
Delta R.T.: 0.009 min
Response: 37102
Conc: 1.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

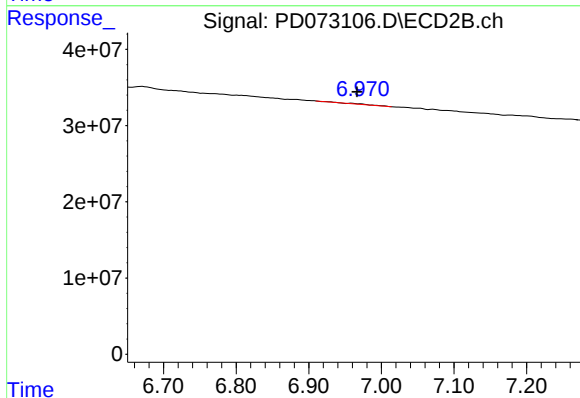


#24 Toxaphene-3

R.T.: 6.960 min
Delta R.T.: -0.007 min
Response: 1544763
Conc: 3.08 ng/ml

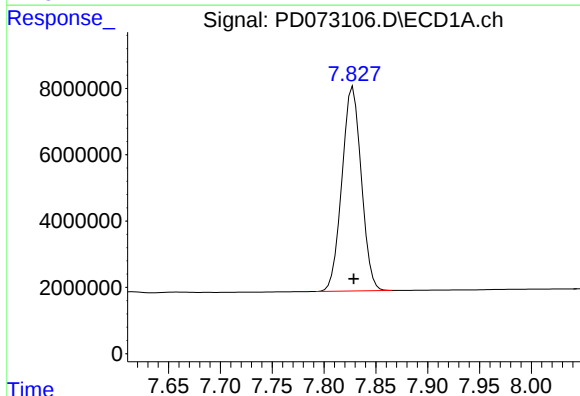

#27 Decachlorobiphenyl

R.T.: 7.828 min
Delta R.T.: 0.000 min
Response: 80076593
Conc: 35.09 ng/ml

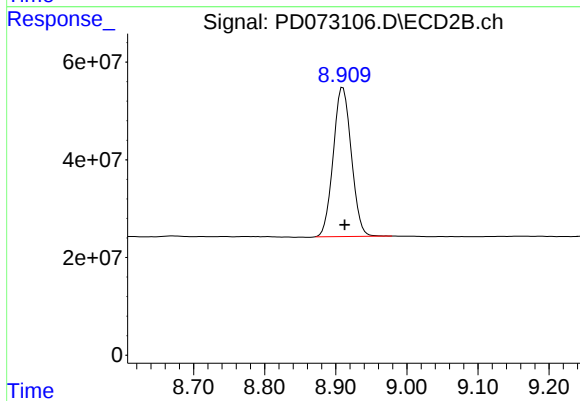

#27 Decachlorobiphenyl

R.T.: 8.910 min
Delta R.T.: -0.003 min
Response: 539698174
Conc: 36.47 ng/ml