

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111922\
 Data File : PD073113.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2022 13:29
 Operator : AR\AJ
 Sample : PB149087BS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS087

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 05:13:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.699	3.459	44365993	1170.8E6	18.502	17.923
27)	SA Decachlor...	7.827	8.911	88993686	597.3E6	39.000	40.363
Target Compounds							
2)	A alpha-BHC	3.201	3.923	15870858	437.6E6	4.337	5.018
3)	MA gamma-BHC...	3.532	4.257	15378573	347.6E6	4.634	5.122
4)	MA Heptachlor	3.864	4.823	15367373	236.0E6	4.600	5.140
5)	MB Aldrin	4.143	5.162	15880992	213.4E6	4.713	5.314
6)	B beta-BHC	3.833	4.472	7618836	148.0E6	4.745	5.538
7)	B delta-BHC	4.063	4.716	15372800	275.2E6	4.230	5.058
8)	B Heptachlo...	4.647	5.594	14995843	174.3E6	4.826	5.158
9)	A Endosulfan I	5.016	5.978	13653796	151.9E6	4.831	5.221
10)	B trans-Chl...	4.896	5.848	14862059	162.4E6	4.822	5.141
11)	B cis-Chlor...	4.959	5.923	14754861	161.8E6	4.712	5.098
12)	B 4,4'-DDE	5.147	6.097	25957889	302.8E6	8.677	10.086
13)	MA Dieldrin	5.282	6.255	28329246	320.4E6	9.248	10.628
14)	MA Endrin	5.559	6.487	24318494	250.5E6	8.970	10.155
15)	B Endosulfa...	5.857	6.717	25369247	261.1E6	9.420	10.810
16)	A 4,4'-DDD	5.706	6.621	22671364	250.8E6	9.410	10.945
17)	MA 4,4'-DDT	5.954	6.929	19178992	216.6E6	8.574	10.086
18)	B Endrin al...	6.039	6.848	21202634	204.1E6	9.817	10.773
19)	B Endosulfa...	6.262	7.081	23524619	213.3E6	9.376	10.256
20)	A Methoxychlor	6.538	7.408	59666958	494.7E6	47.640	53.018
21)	B Endrin ke...	6.772	7.570	29770064	247.7E6	10.198	11.095

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111922\
Data File : PD073113.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2022 13:29
Operator : AR\AJ
Sample : PB149087BS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 05:13:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

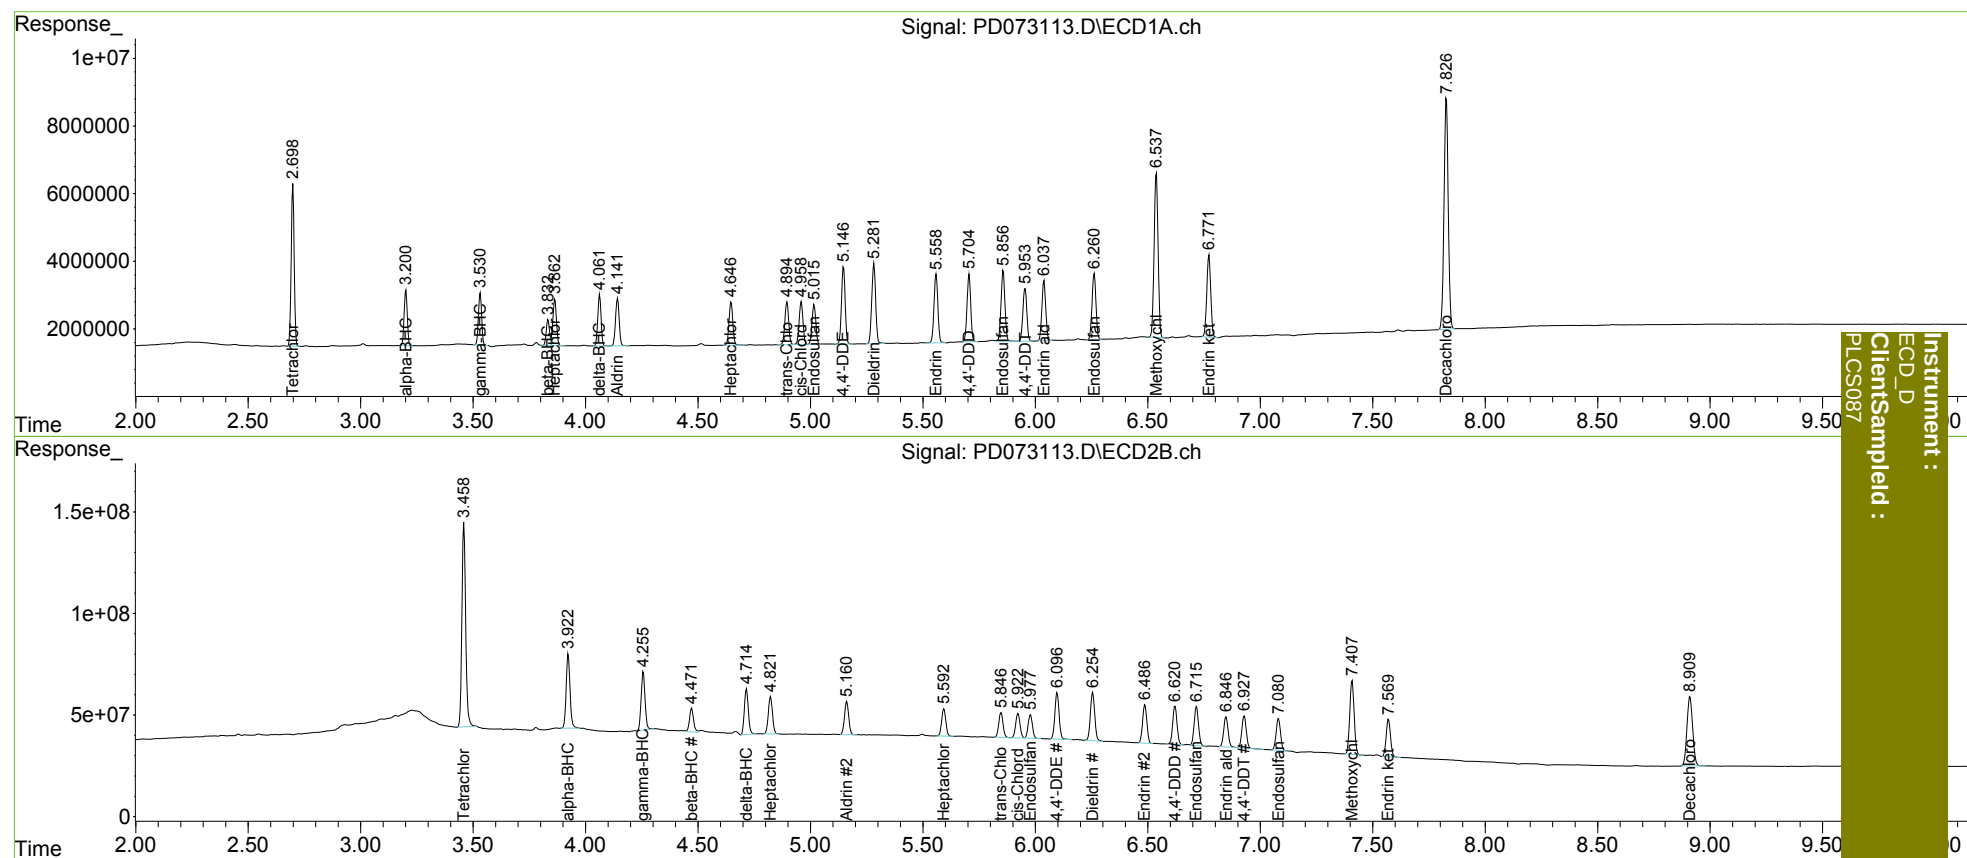

Instrument :
ECD_D
ClientSampled :
PLCS087