

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111922\
 Data File : PD073123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2022 15:42
 Operator : AR\AJ
 Sample : INDA380
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3228

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 05:20:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.698	3.459	43110135	1212.4E6	17.978	18.560
27)	SA Decachlor...	7.827	8.911	82238612	559.9E6	36.040	37.835
Target Compounds							
2)	A alpha-BHC	3.201	3.923	65416394	1582.8E6	17.874	18.150
3)	MA gamma-BHC...	3.531	4.256	60669674	1235.9E6	18.281	18.215
4)	MA Heptachlor	3.864	4.822	58898139	831.9E6	17.630	18.116
9)	A Endosulfan I	5.016	5.978	50479035	540.4E6	17.862	18.576
13)	MA Dieldrin	5.282	6.254	110.2E6	1122.3E6	35.970	37.234
14)	MA Endrin	5.559	6.486	91421718	875.1E6	33.722	35.478
16)	A 4,4'-DDD	5.705	6.620	89840226	897.4E6	37.289	39.157
17)	MA 4,4'-DDT	5.954	6.928	76049948	768.1E6	33.997	35.762
20)	A Methoxychlor	6.537	7.408	216.6E6	1705.2E6	172.923	182.754

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD111922\
Data File : PD073123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2022 15:42
Operator : AR\AJ
Sample : INDA380
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 05:20:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

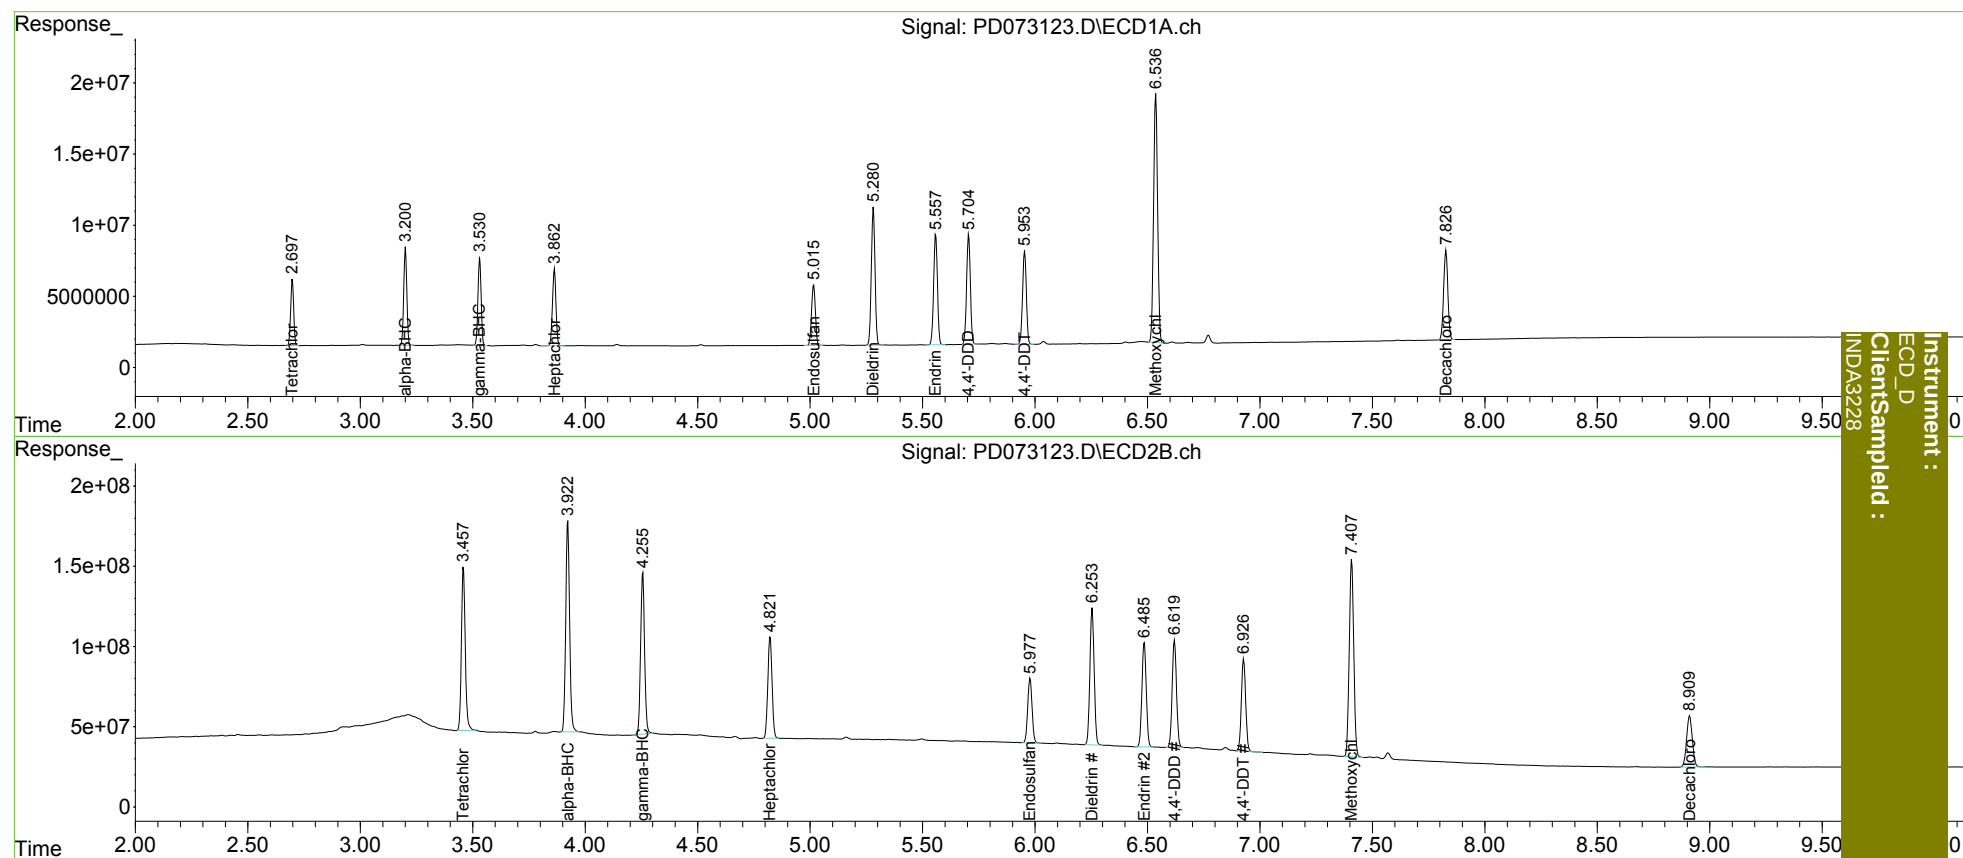

Instrument :
ECD_D
ClientSampled :
INDA3228