

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112018\
 Data File : PD050445.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Nov 2018 8:28
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 10:40:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111918CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Nov 19 17:32:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds


8) B	Heptachlo...	0.000	5.924	0	233.5E6	N.D.	6.753
------	--------------	-------	-------	---	---------	------	-------


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112018\
Data File : PD050445.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Nov 2018 8:28
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 10:40:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111918CLP.M
Quant Title : GC Extractables
QLast Update : Mon Nov 19 17:32:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

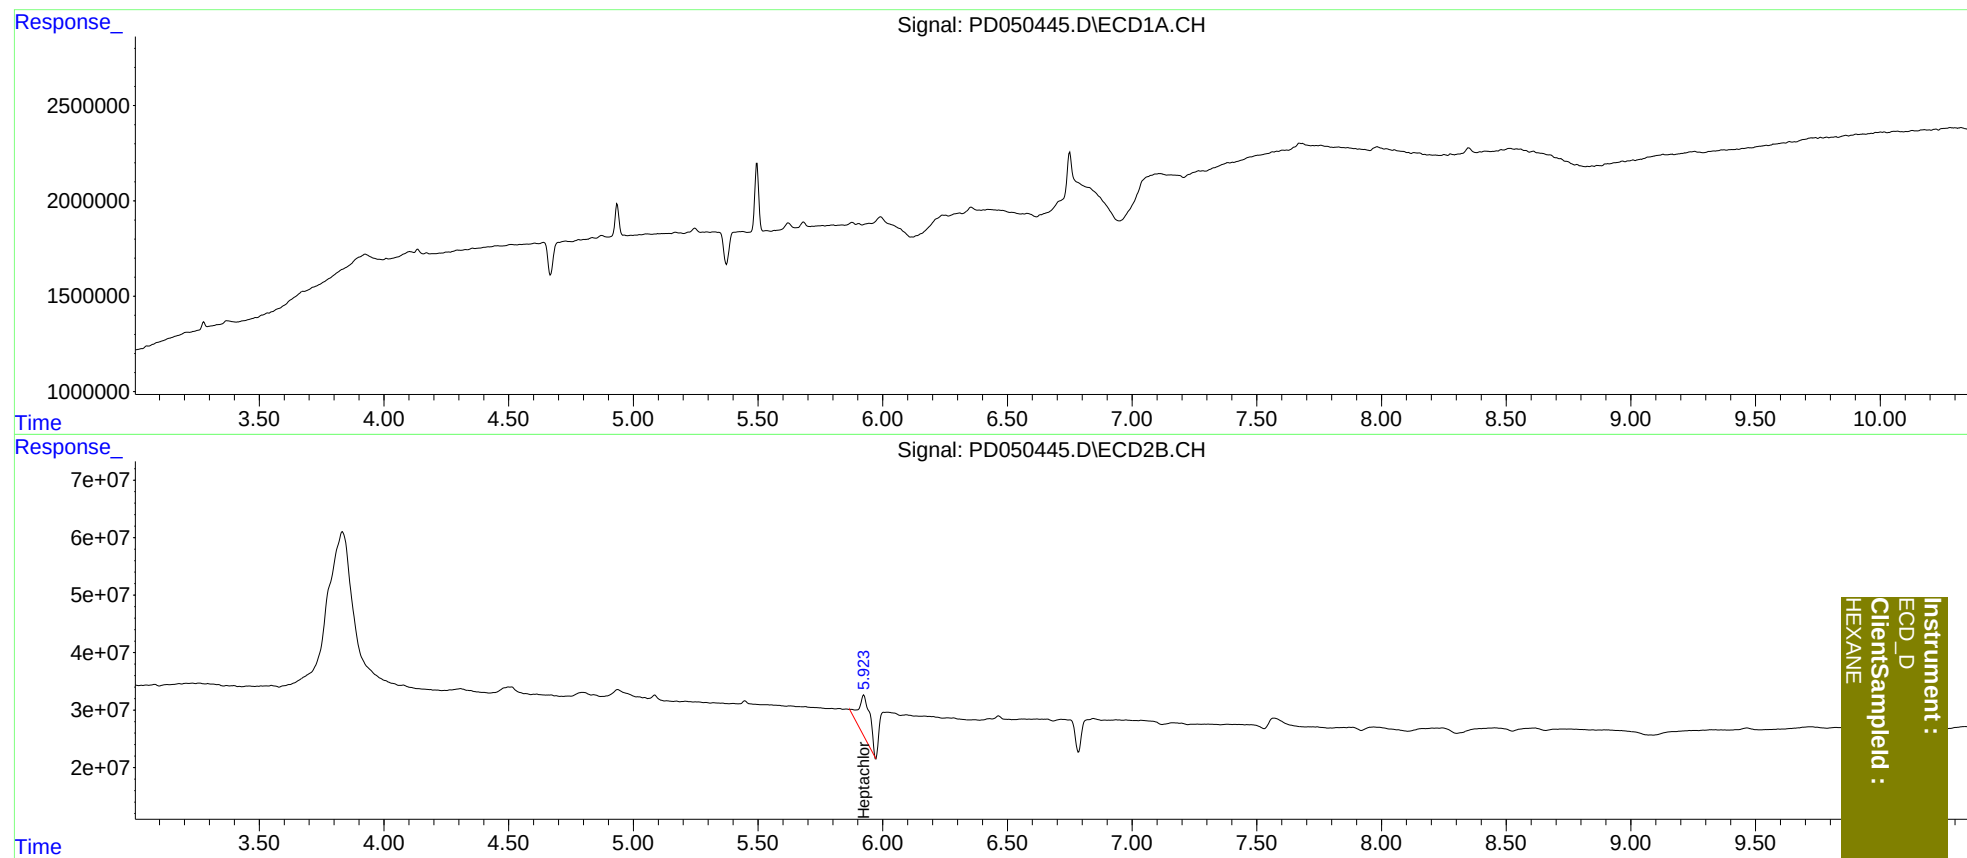


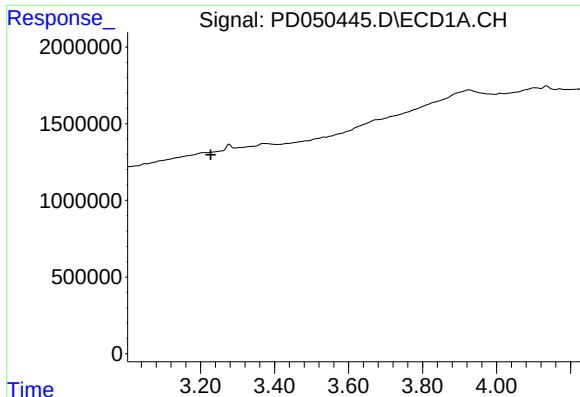

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.228 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

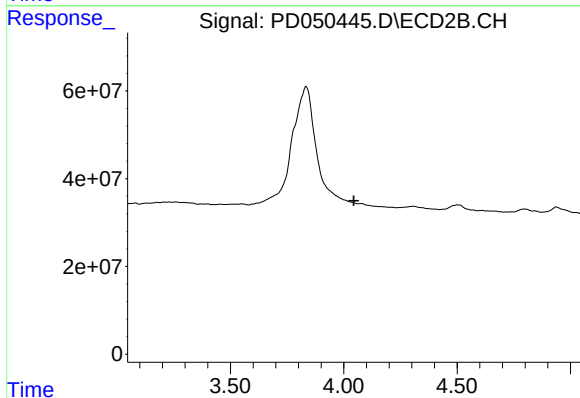


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.044 min
Response: 0
Conc: N.D.

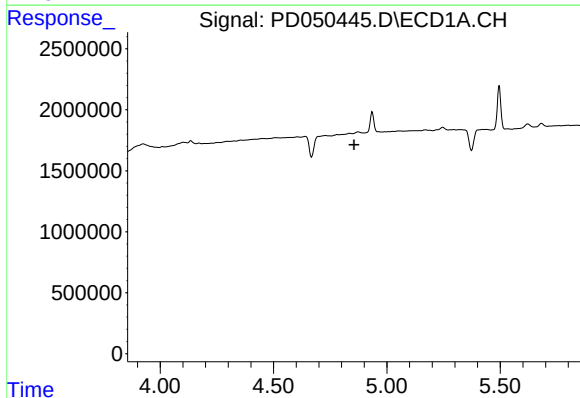


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.856 min
Response: 0
Conc: N.D.

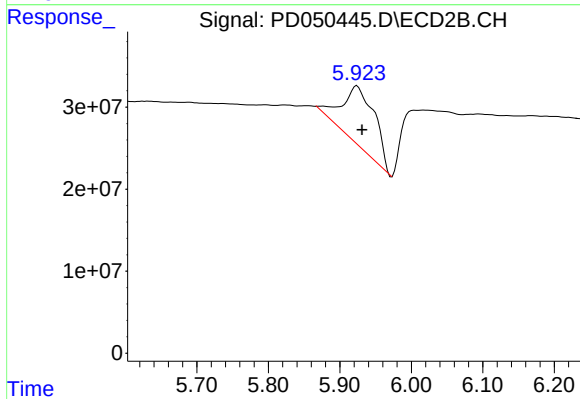

#8 Heptachlor epoxide


R.T.: 5.924 min
Delta R.T.: -0.007 min
Response: 233473159
Conc: 6.75 ng/ml

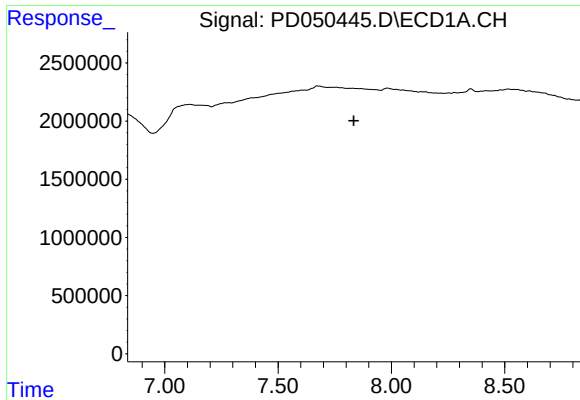

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.834 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

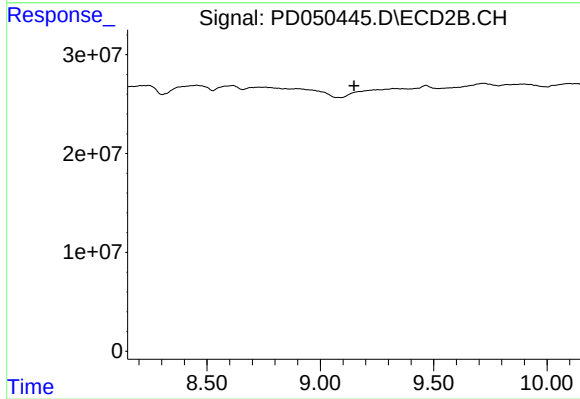

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.149 min
Response: 0
Conc: N.D.