

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112018\
 Data File : PD050458.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Nov 2018 13:33
 Operator : AJ\SJ
 Sample : PIBLK47
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK47

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 06:40:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111918CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Nov 19 17:32:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.228	4.044	29586715	604.5E6	18.690	18.773
2) SA Decachlor...	7.835	9.152	58883475	749.3E6	30.038	37.714 #
Target Compounds						
7) B delta-BHC	0.000	5.088	0 12714839	N.D.	0.298	
8) B Heptachlo...	0.000	6.001f	0 46827845	N.D.	1.354	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112018\
Data File : PD050458.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Nov 2018 13:33
Operator : AJ\SJ
Sample : PIBLK47
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 06:40:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111918CLP.M
Quant Title : GC Extractables
QLast Update : Mon Nov 19 17:32:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

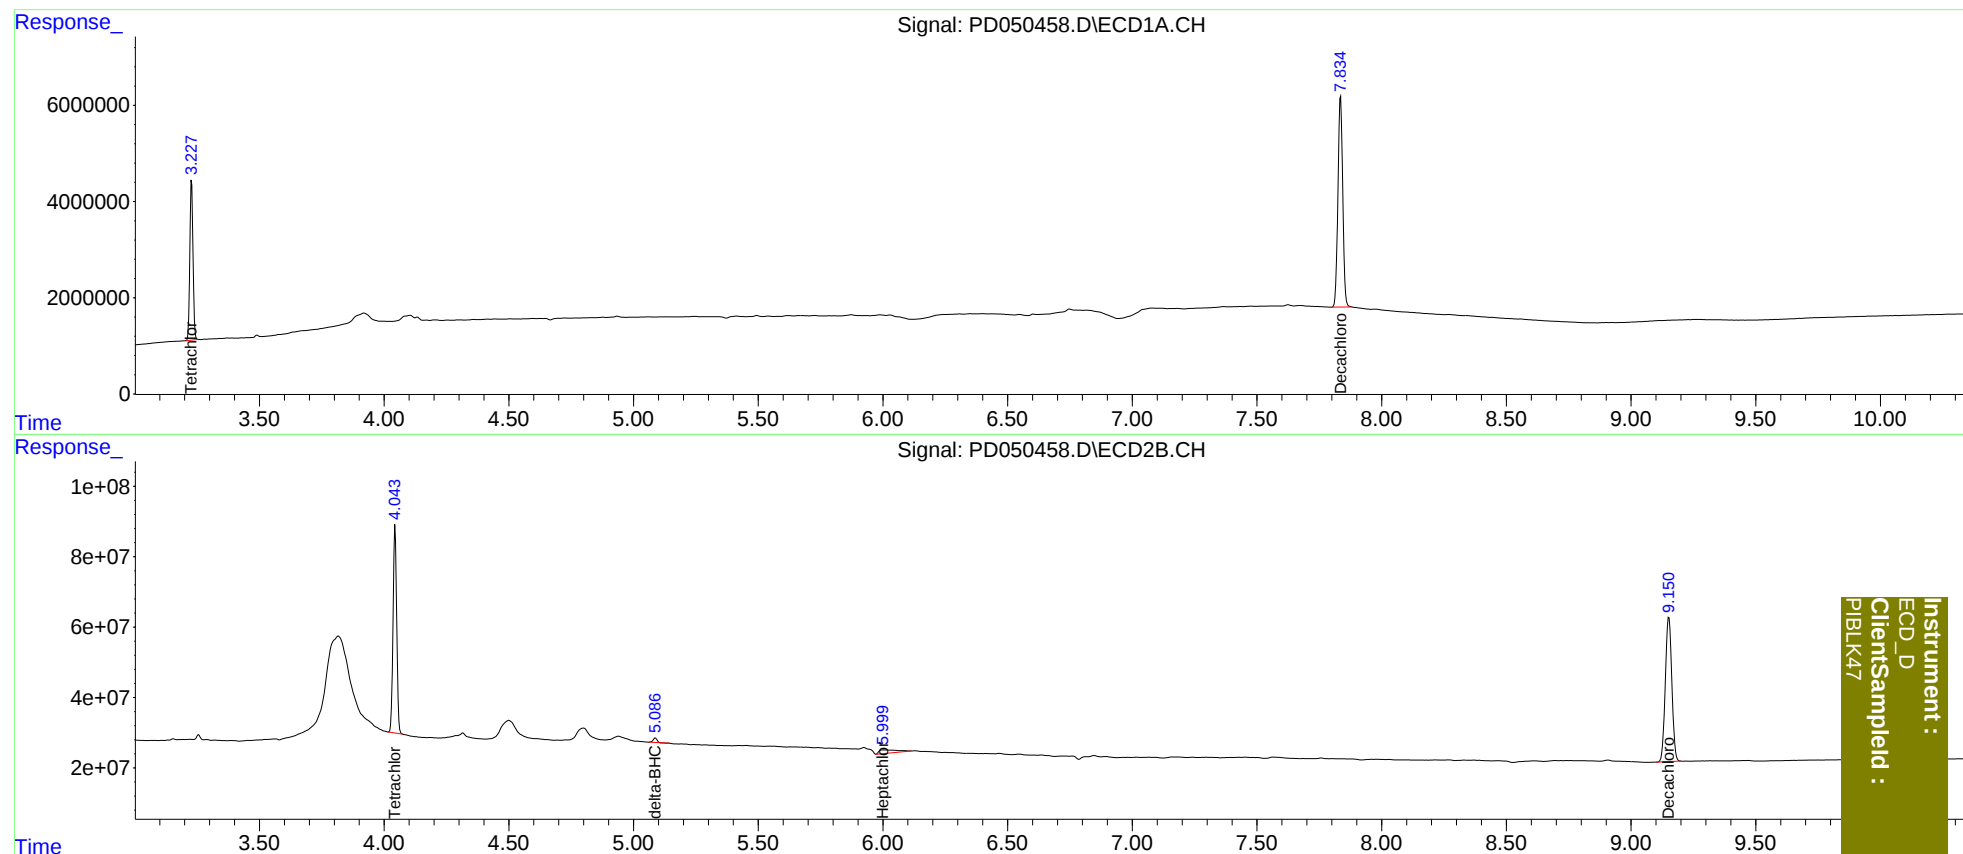


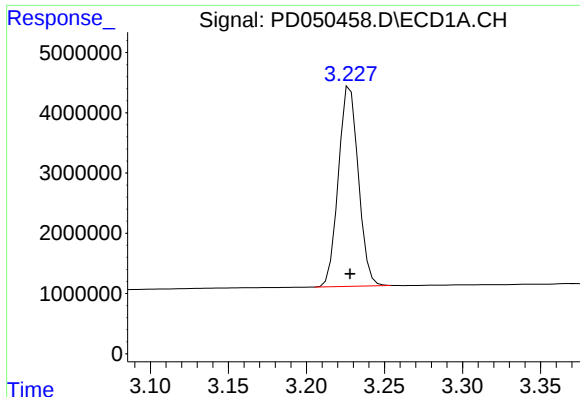

#1 Tetrachloro-m-xylene


R.T.: 3.228 min
Delta R.T.: 0.000 min
Response: 29586715
Conc: 18.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK47

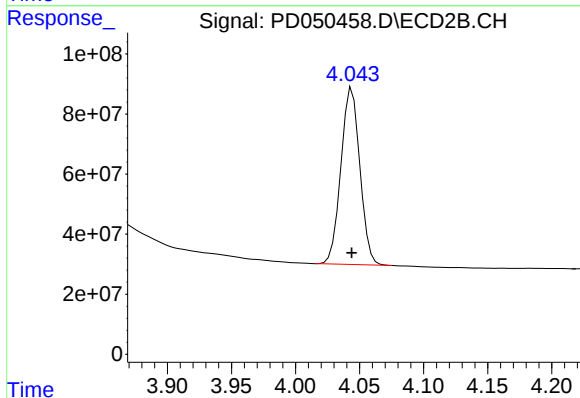


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 604463741
Conc: 18.77 ng/ml

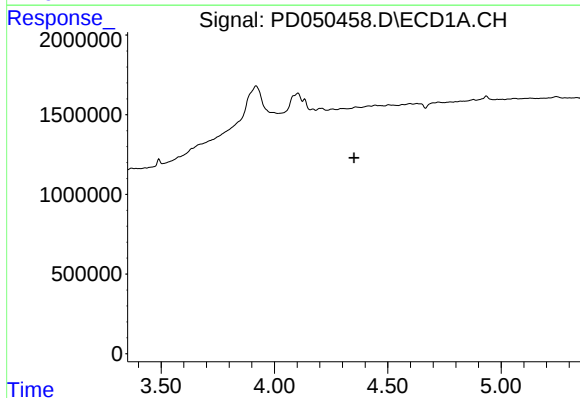


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.351 min
Response: 0
Conc: N.D.

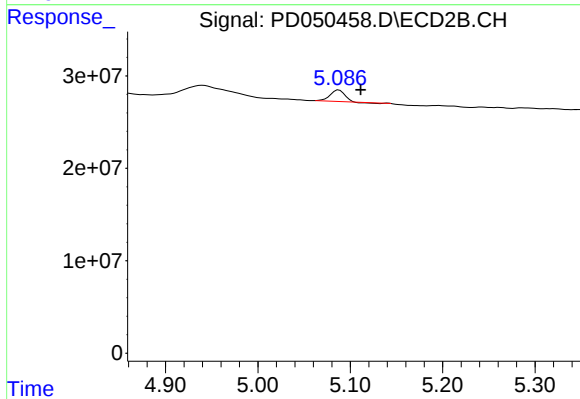

#7 delta-BHC


R.T.: 5.088 min
Delta R.T.: -0.023 min
Response: 12714839
Conc: 0.30 ng/ml

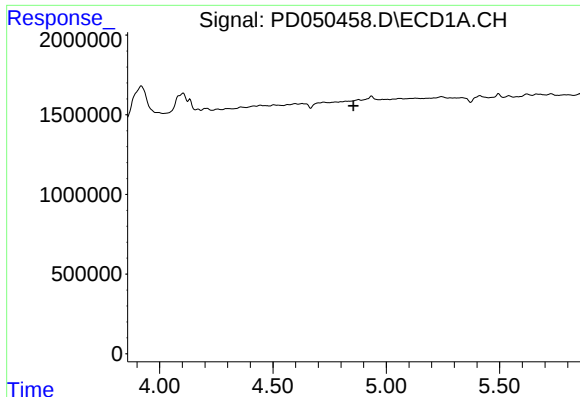

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.856 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK47

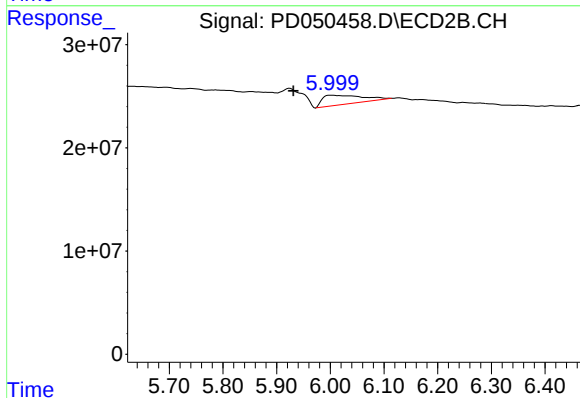


#8 Heptachlor epoxide

R.T.: 6.001 min
Delta R.T.: 0.070 min
Response: 46827845
Conc: 1.35 ng/ml

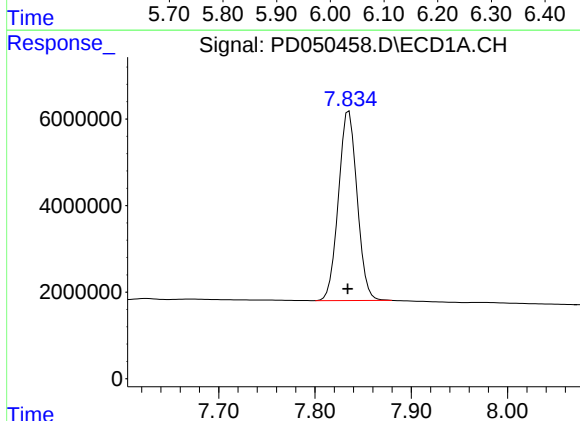

#27 Decachlorobiphenyl

R.T.: 7.835 min
Delta R.T.: 0.001 min
Response: 58883475
Conc: 30.04 ng/ml

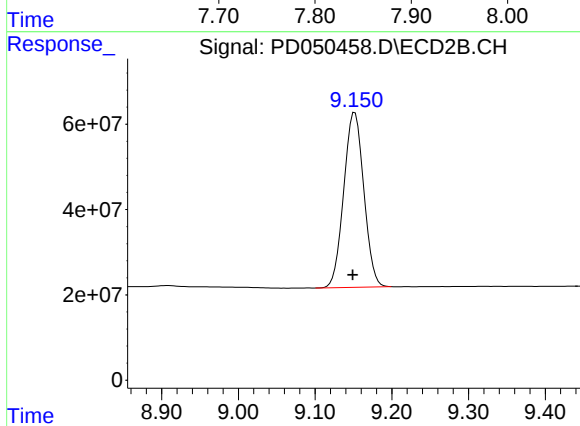

#27 Decachlorobiphenyl

R.T.: 9.152 min
Delta R.T.: 0.003 min
Response: 749326725
Conc: 37.71 ng/ml