

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112018\
 Data File : PD050463.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Nov 2018 15:24
 Operator : AJ\SJ
 Sample : J5990-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ETO74

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 06:41:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111918CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Nov 19 17:32:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	4.044	25402187	499.1E6	16.047	15.500
27)	SA Decachlor...	7.835	9.151	27038193	345.5E6	13.793	17.392 #


Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112018\
Data File : PD050463.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Nov 2018 15:24
Operator : AJ\SJ
Sample : J5990-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 06:41:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111918CLP.M
Quant Title : GC Extractables
QLast Update : Mon Nov 19 17:32:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

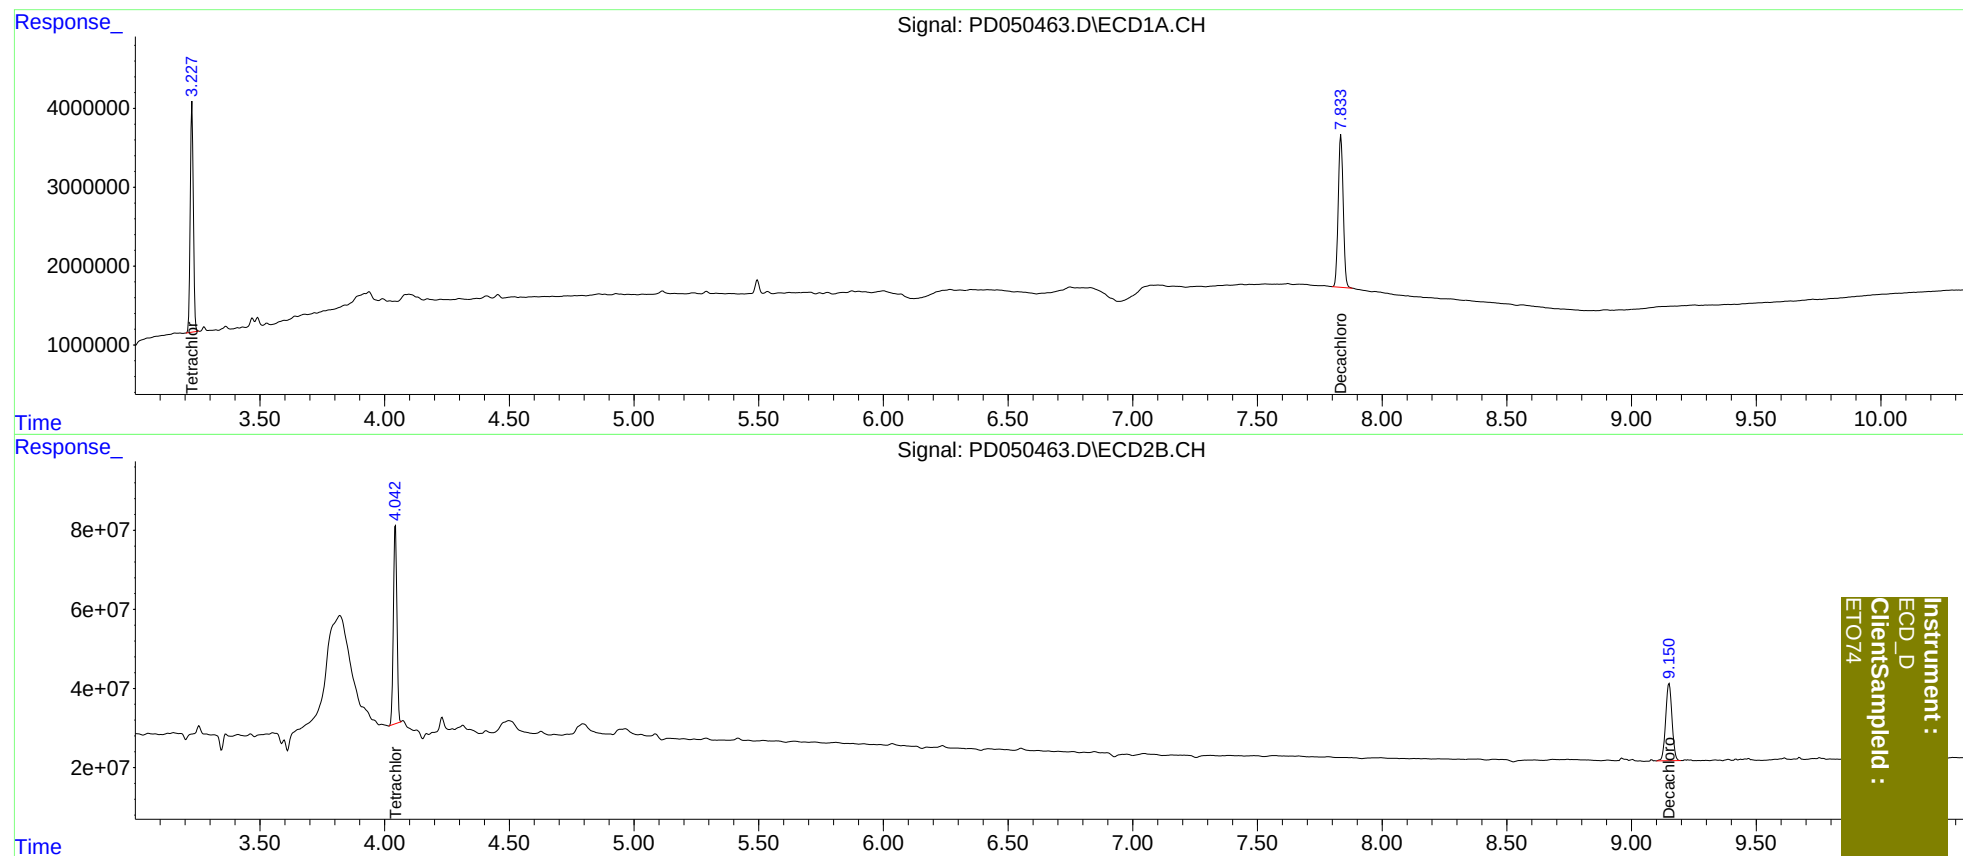


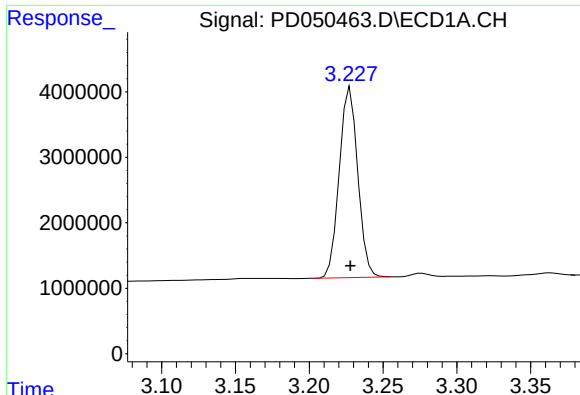

#1 Tetrachloro-m-xylene


R.T.: 3.228 min
Delta R.T.: 0.000 min
Response: 25402187
Conc: 16.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
ETO74

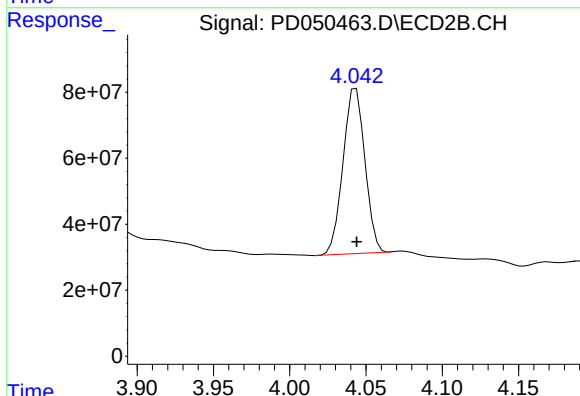


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 499098283
Conc: 15.50 ng/ml

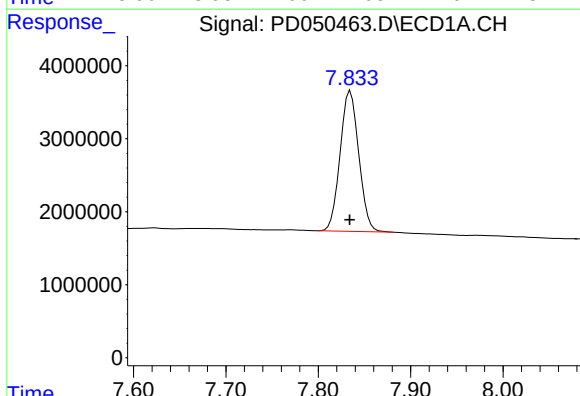

#27 Decachlorobiphenyl

R.T.: 7.835 min
Delta R.T.: 0.000 min
Response: 27038193
Conc: 13.79 ng/ml

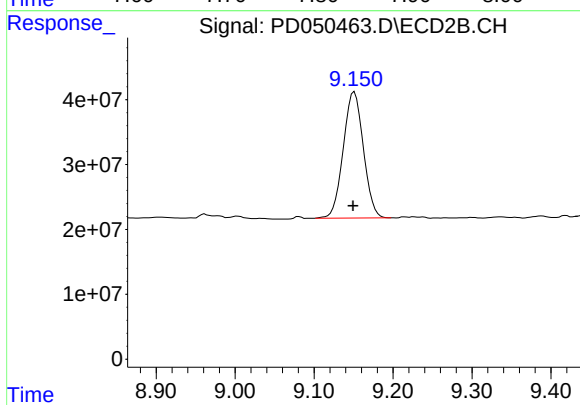

#27 Decachlorobiphenyl

R.T.: 9.151 min
Delta R.T.: 0.002 min
Response: 345547375
Conc: 17.39 ng/ml