

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112019\
 Data File : PD056123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2019 17:48
 Operator : SG\AJ
 Sample : K5888-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JLLP7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 00:56:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.288	3.962	15783652	22544689	20.967	21.513
27) SA	Decachlor...	7.962	8.997	26392883	31019119	32.379	27.316
Target Compounds							
3) MA	gamma-BHC...	0.000	4.595f	0	143172	N.D.	0.102
6) B	beta-BHC	0.000	4.849f	0	1006351	N.D.	1.438
9) A	Endosulfan I	0.000	6.135f	0	602904	N.D.	0.463
10) B	trans-Chl...	0.000	6.025	0	641185	N.D.	0.449
11) B	cis-Chlor...	0.000	6.135	0	602904	N.D.	0.430
13) MA	Dieldrin	0.000	6.378f	0	109082	N.D.	<MDL
15) B	Endosulfa...	0.000	6.873	0	248030	N.D.	0.192
19) B	Endosulfa...	0.000	7.238	0	252588	N.D.	0.210
22)	Toxaphene-1	0.000	6.378	0	109082	N.D.	10.624


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112019\
Data File : PD056123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2019 17:48
Operator : SG\AJ
Sample : K5888-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
JLLP7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 00:56:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

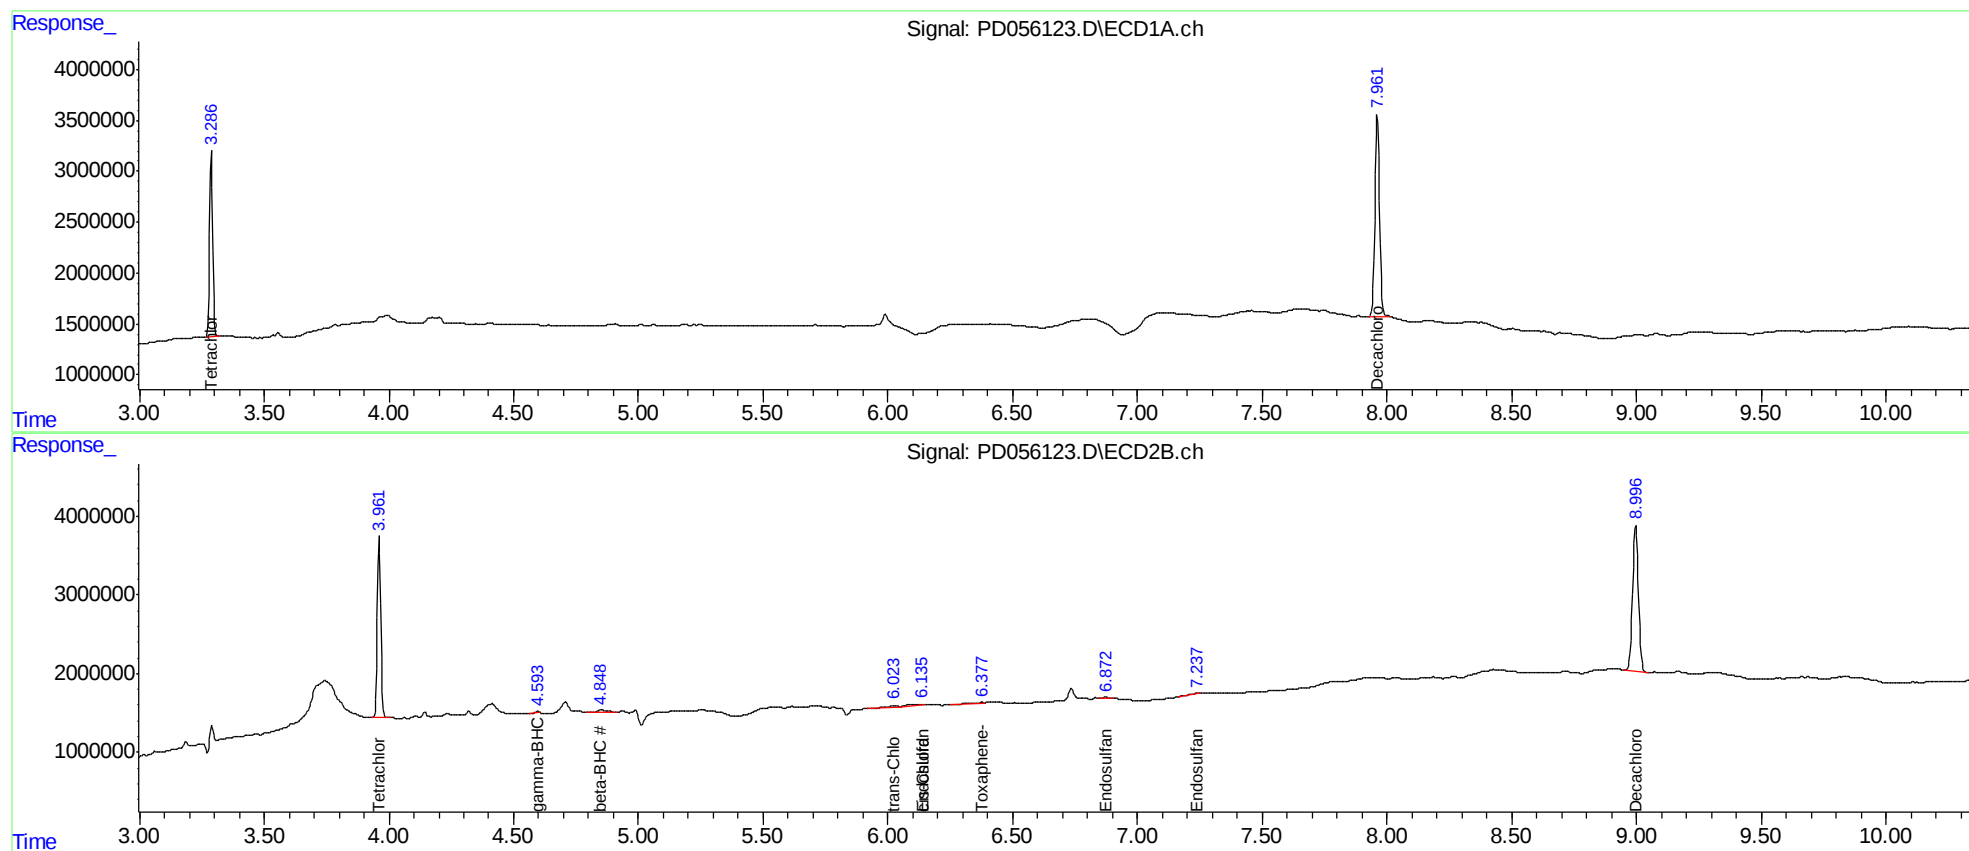


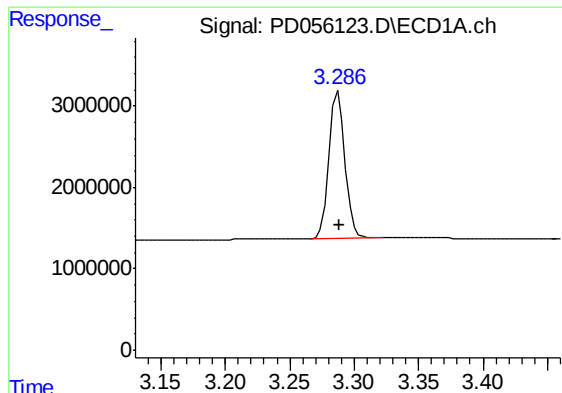

#1 Tetrachloro-m-xylene


R.T.: 3.288 min
Delta R.T.: -0.001 min
Response: 15783652
Conc: 20.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
JLLP7

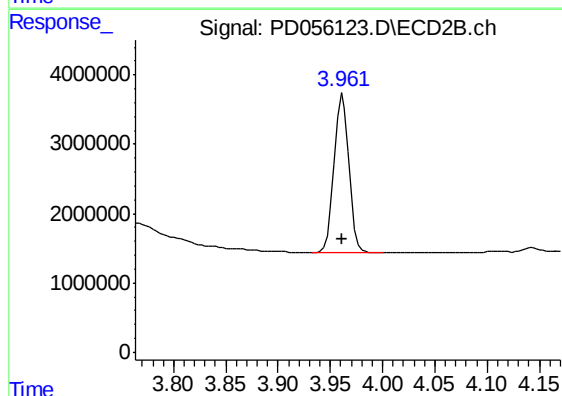


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 22544689
Conc: 21.51 ng/ml

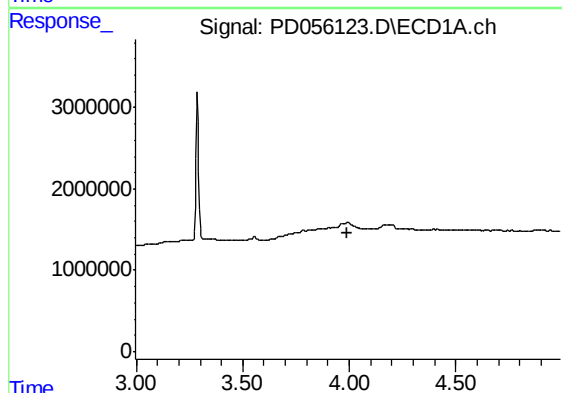


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.991 min
Response: 0
Conc: N.D.

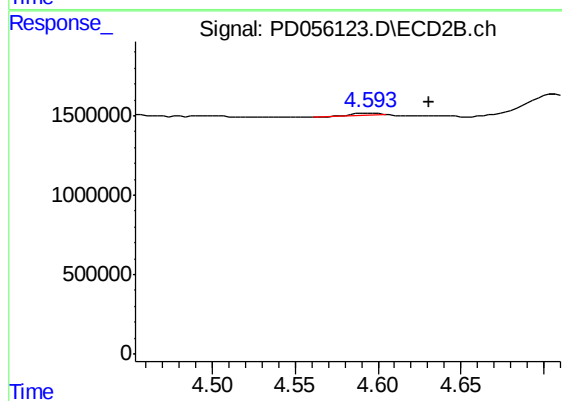

#3 gamma-BHC (Lindane)


R.T.: 4.595 min
Delta R.T.: -0.036 min
Response: 143172
Conc: 0.10 ng/ml

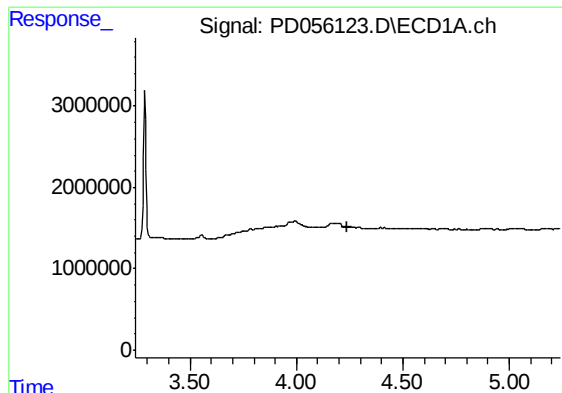

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.240 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
JLLP7

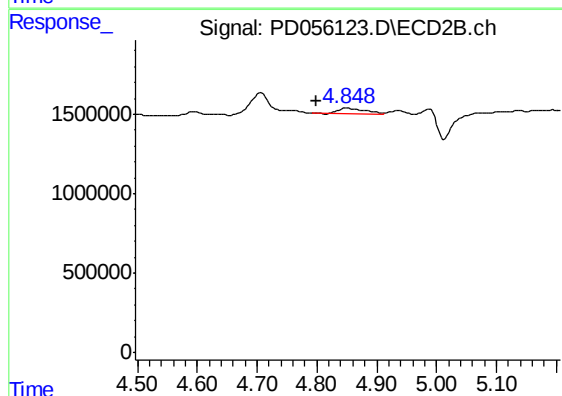


#6 beta-BHC

R.T.: 4.849 min
Delta R.T.: 0.050 min
Response: 1006351
Conc: 1.44 ng/ml

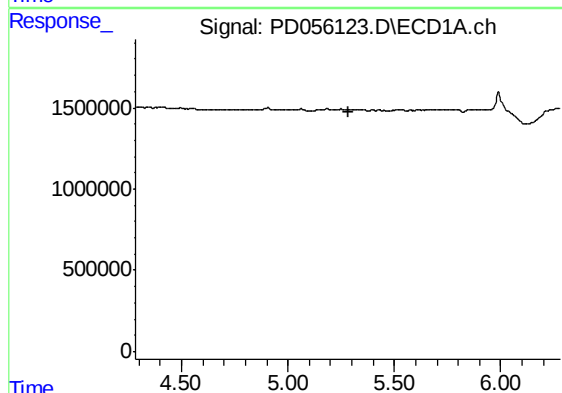


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.283 min
Response: 0
Conc: N.D.

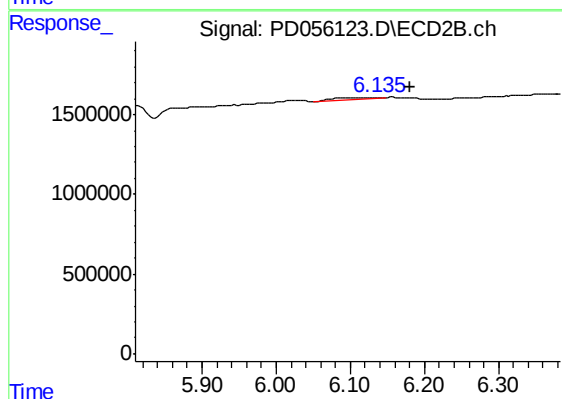

#9 Endosulfan I


R.T.: 6.135 min
Delta R.T.: -0.045 min
Response: 602904
Conc: 0.46 ng/ml

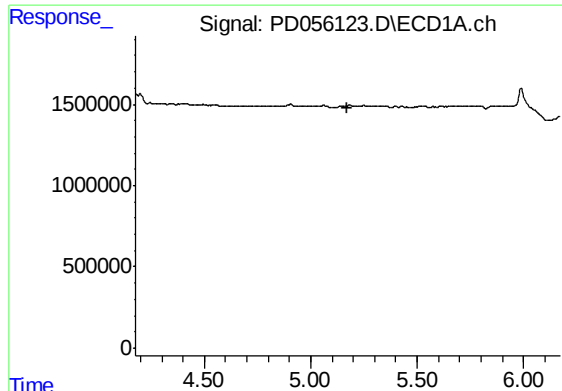

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
JLLP7

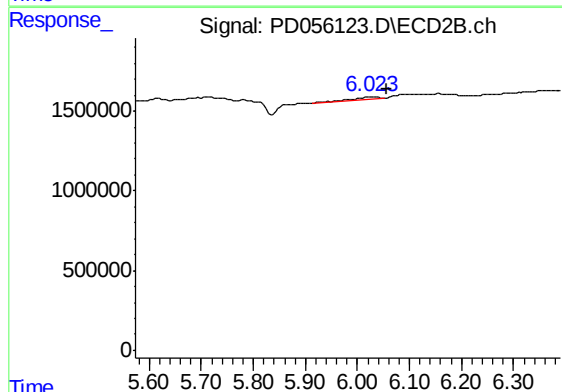


#10 trans-Chlordane

R.T.: 6.025 min
Delta R.T.: -0.033 min
Response: 641185
Conc: 0.45 ng/ml

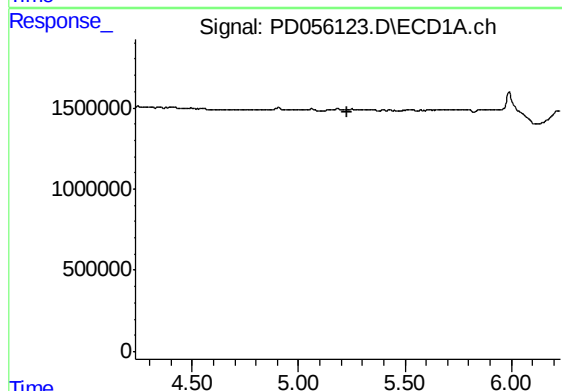


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.231 min
Response: 0
Conc: N.D.

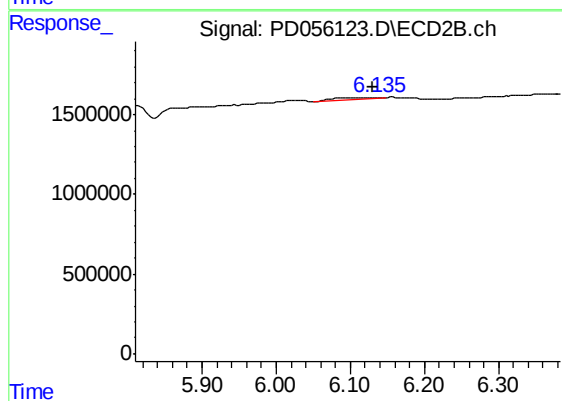

#11 cis-Chlordane


R.T.: 6.135 min
Delta R.T.: 0.005 min
Response: 602904
Conc: 0.43 ng/ml

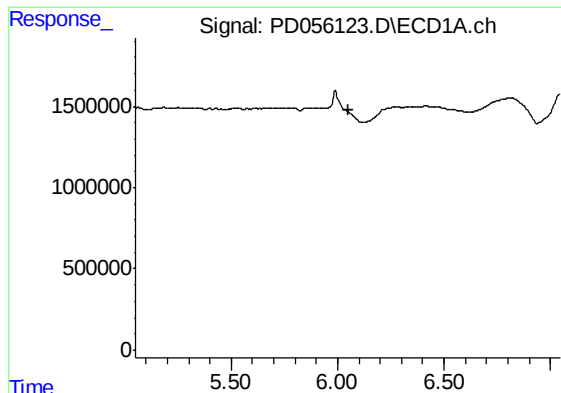

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
JLLP7

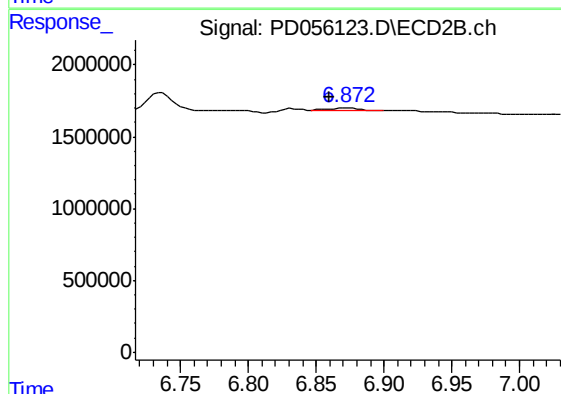


#15 Endosulfan II

R.T.: 6.873 min
Delta R.T.: 0.013 min
Response: 248030
Conc: 0.19 ng/ml

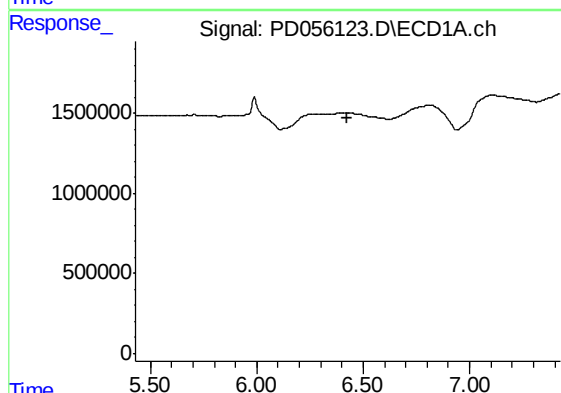


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

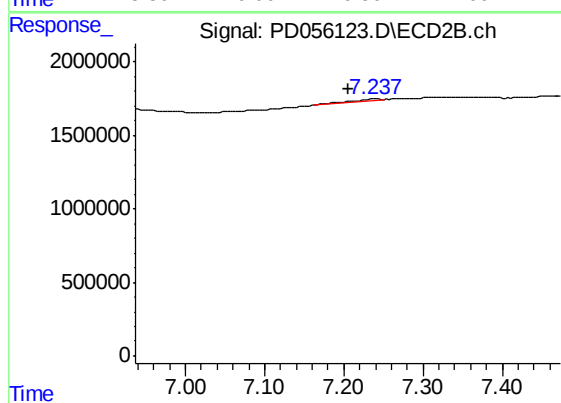

#19 Endosulfan Sulfate


R.T.: 7.238 min
Delta R.T.: 0.032 min
Response: 252588
Conc: 0.21 ng/ml

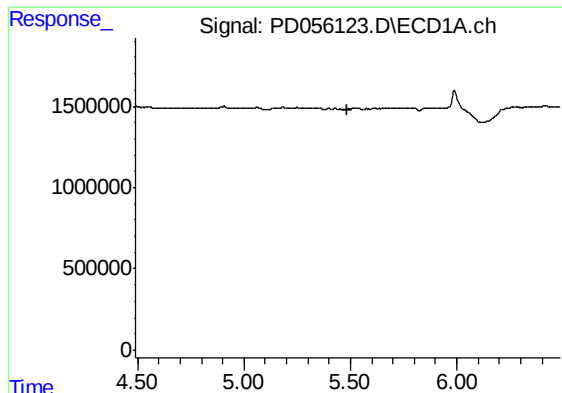

#22 Toxaphene-1


R.T.: 0.000 min
Exp R.T.: 5.488 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
JLLP7

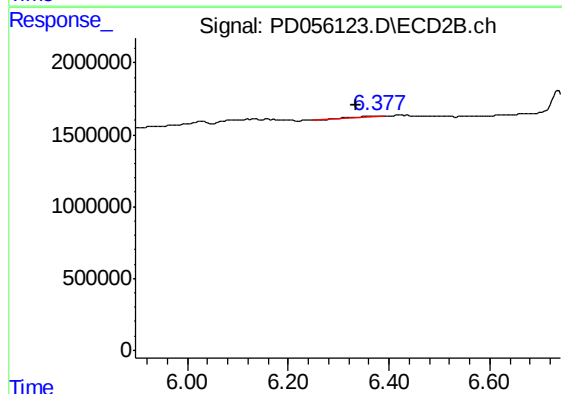


#22 Toxaphene-1

R.T.: 6.378 min
Delta R.T.: 0.043 min
Response: 109082
Conc: 10.62 ng/ml

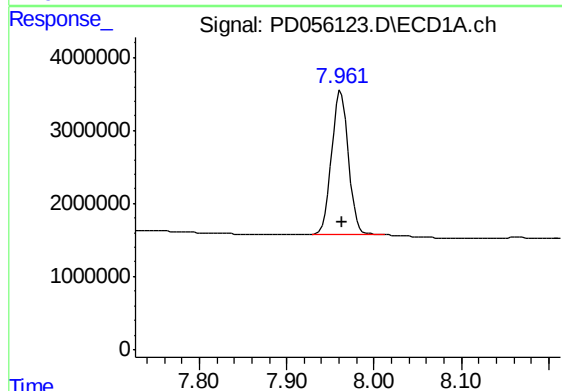

#27 Decachlorobiphenyl

R.T.: 7.962 min
Delta R.T.: 0.000 min
Response: 26392883
Conc: 32.38 ng/ml

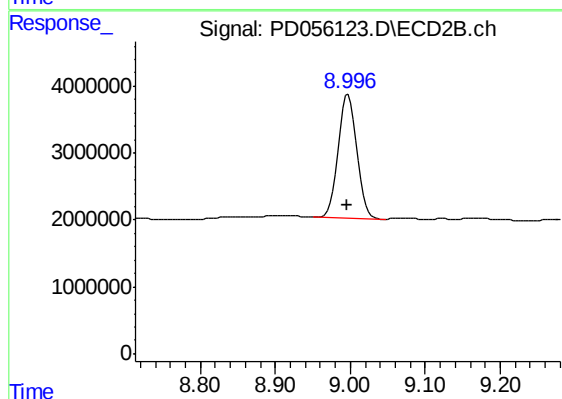

#27 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: 0.000 min
Response: 31019119
Conc: 27.32 ng/ml