

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112019\
 Data File : PD056130.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2019 19:26
 Operator : SG\AJ
 Sample : K5888-09
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JLLQ9

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 00:57:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.962	12274237	17142825	16.305	16.358
27)	SA Decachlor...	7.962	8.997	20282512	25172421	24.883	22.167
Target Compounds							
6)	B beta-BHC	0.000	4.767f	0	45853	N.D.	<MDL
10)	B trans-Chl...	0.000	6.027	0	335212	N.D.	0.235
11)	B cis-Chlor...	0.000	6.099	0	316173	N.D.	0.225
15)	B Endosulfa...	0.000	6.873	0	960273	N.D.	0.742
16)	A 4,4'-DDD	0.000	6.735f	0	356906	N.D.	0.320
20)	A Methoxychlor	0.000	7.531	0	110909	N.D.	0.178


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112019\
Data File : PD056130.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2019 19:26
Operator : SG\AJ
Sample : K5888-09
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
JLLQ9

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 00:57:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

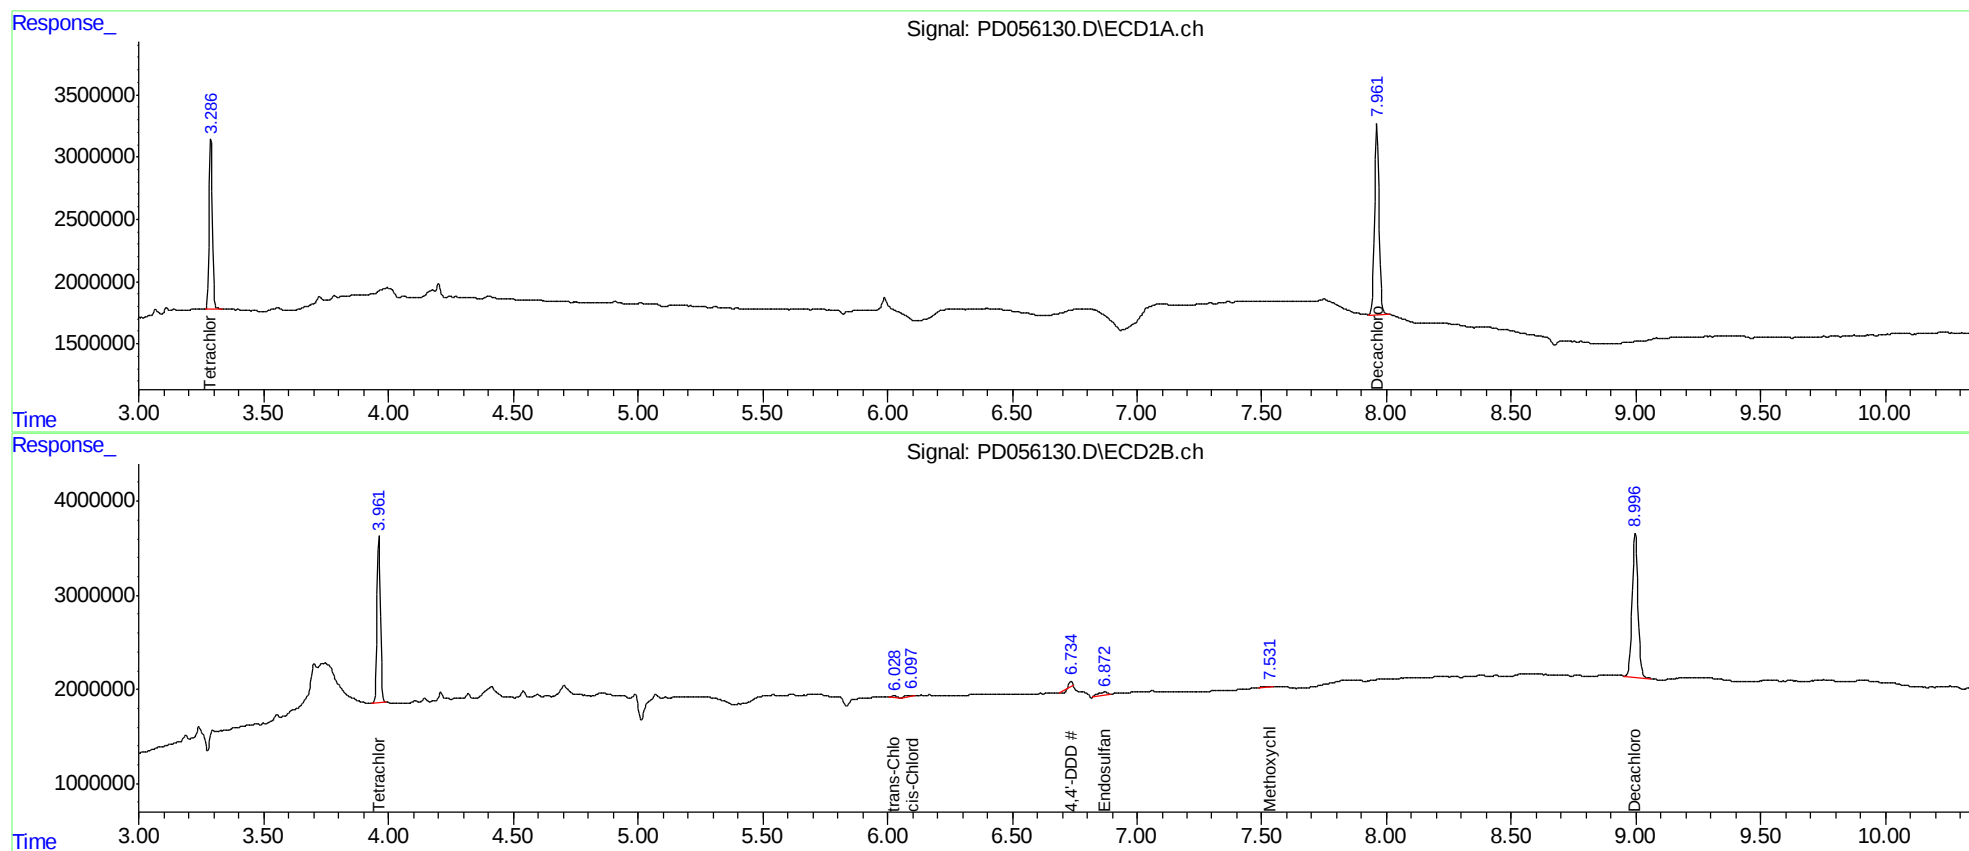


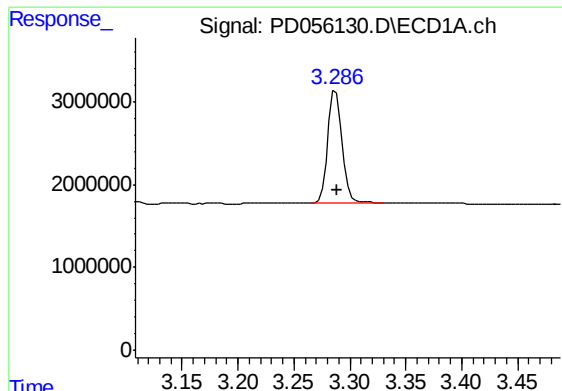

#1 Tetrachloro-m-xylene


R.T.: 3.288 min
Delta R.T.: -0.001 min
Response: 12274237
Conc: 16.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
JLLQ9

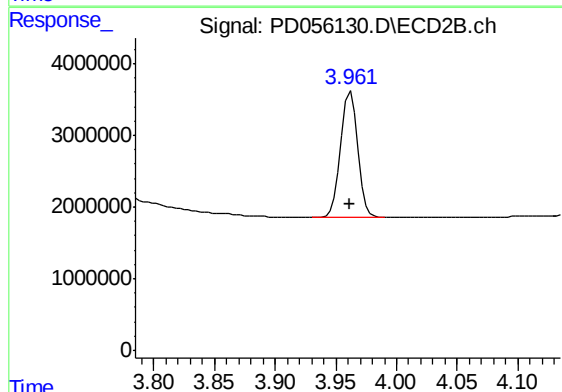


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 17142825
Conc: 16.36 ng/ml

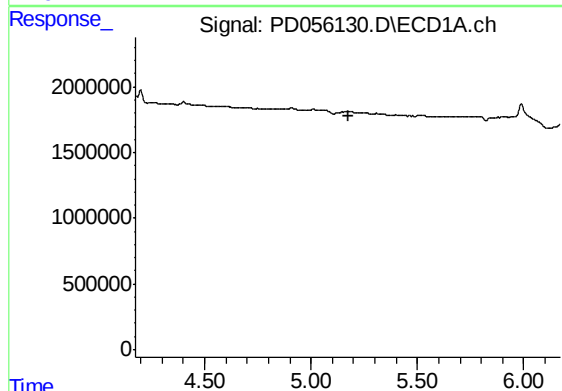


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

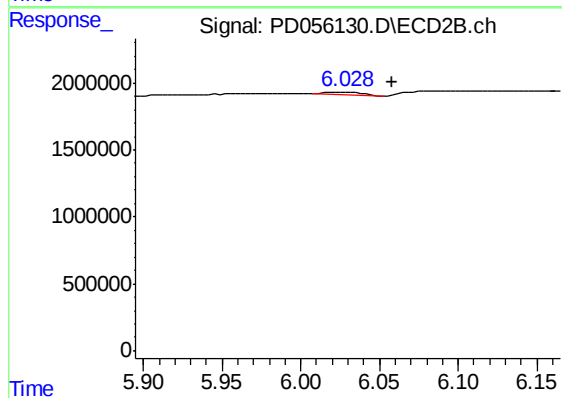

#10 trans-Chlordane


R.T.: 6.027 min
Delta R.T.: -0.031 min
Response: 335212
Conc: 0.23 ng/ml

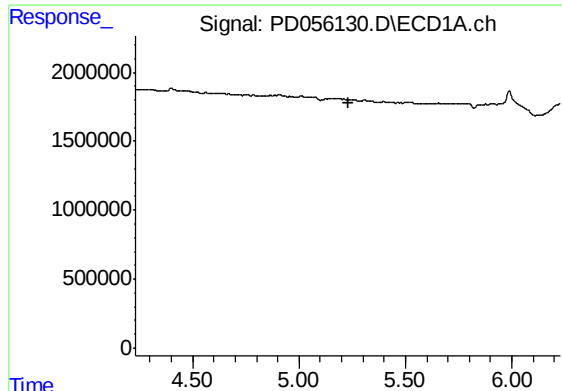

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
JLLQ9

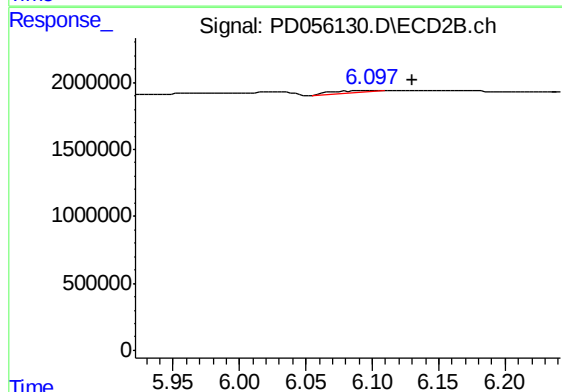


#11 cis-Chlordane

R.T.: 6.099 min
Delta R.T.: -0.031 min
Response: 316173
Conc: 0.23 ng/ml

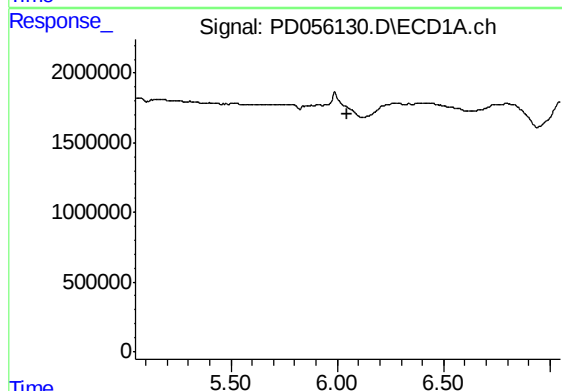


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.049 min
Response: 0
Conc: N.D.

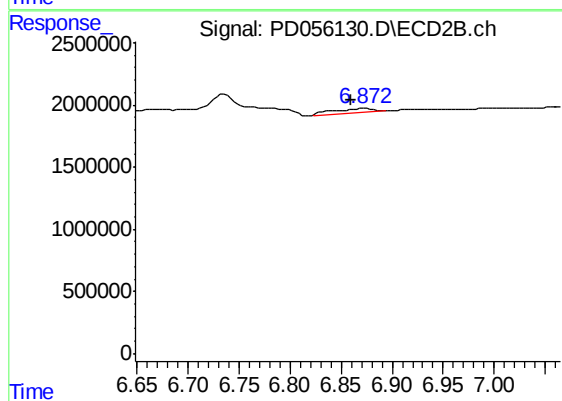

#15 Endosulfan II


R.T.: 6.873 min
Delta R.T.: 0.013 min
Response: 960273
Conc: 0.74 ng/ml

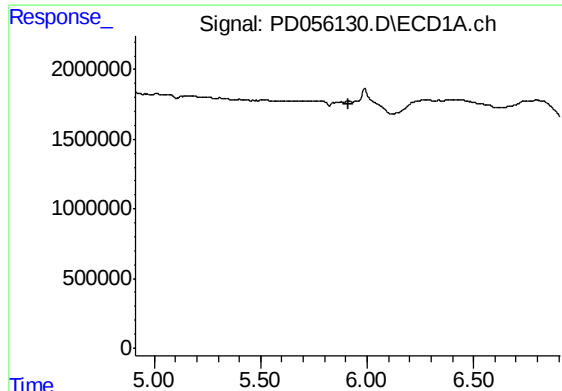

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 5.911 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
JLLQ9

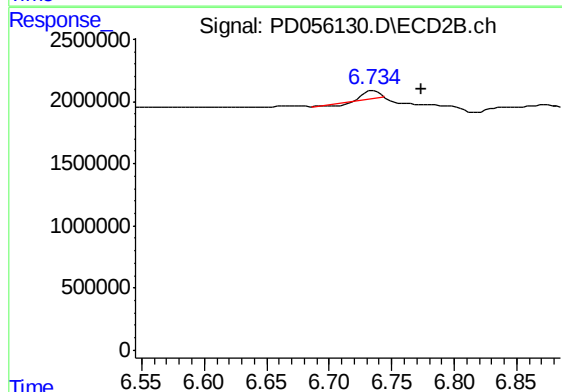


#16 4,4'-DDD

R.T.: 6.735 min
Delta R.T.: -0.039 min
Response: 356906
Conc: 0.32 ng/ml

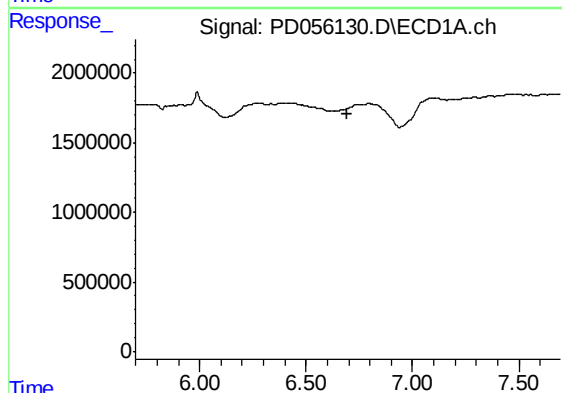


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.695 min
Response: 0
Conc: N.D.

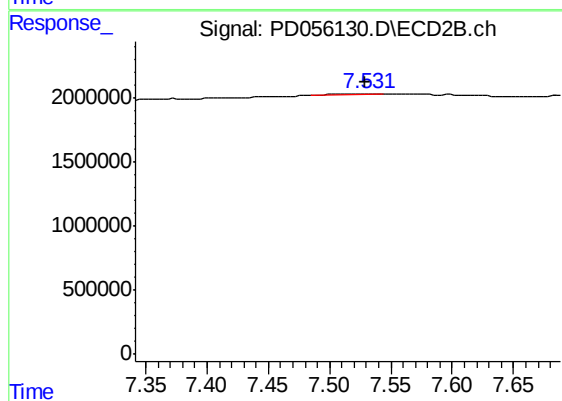

#20 Methoxychlor


R.T.: 7.531 min
Delta R.T.: 0.003 min
Response: 110909
Conc: 0.18 ng/ml

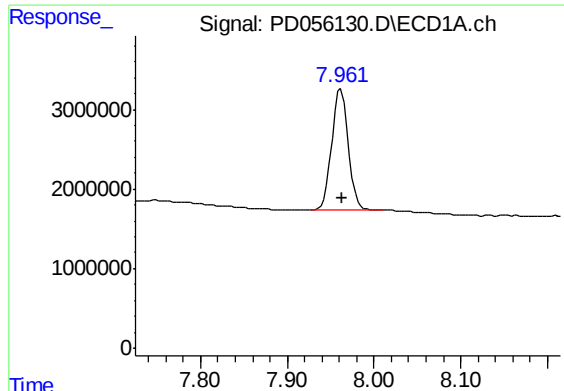

#27 Decachlorobiphenyl

R.T.: 7.962 min
Delta R.T.: -0.001 min
Response: 20282512
Conc: 24.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
JLLQ9

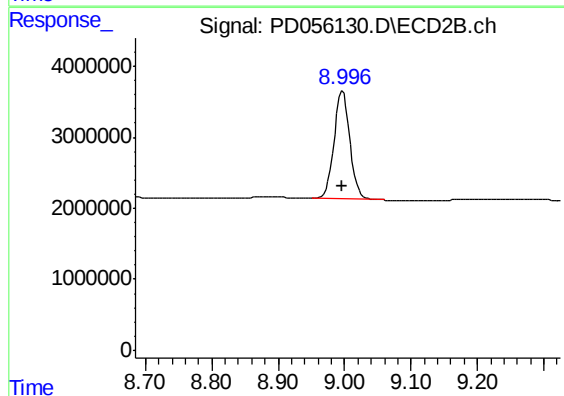

#27 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: 0.000 min
Response: 25172421
Conc: 22.17 ng/ml