

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112019\
 Data File : PD056138.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2019 21:18
 Operator : SG\AJ
 Sample : K5888-17
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JLLP2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 00:59:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.962	13425103	19337917	17.834	18.453
27)	SA Decachlor...	7.962	8.998	22200009	26780347	27.235	23.583
Target Compounds							
3)	MA gamma-BHC...	0.000	4.596f	0	134895	N.D.	<MDL
6)	B beta-BHC	0.000	4.849f	0	1590754	N.D.	2.274
10)	B trans-Chl...	0.000	6.023f	0	619416	N.D.	0.434
11)	B cis-Chlor...	0.000	6.105	0	232578	N.D.	0.166
15)	B Endosulfa...	0.000	6.875	0	357714	N.D.	0.276
16)	A 4,4'-DDD	0.000	6.735f	0	299168	N.D.	0.268
20)	A Methoxychlor	0.000	7.469f	0	53917	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112019\
Data File : PD056138.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2019 21:18
Operator : SG\AJ
Sample : K5888-17
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
JLLP2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 00:59:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

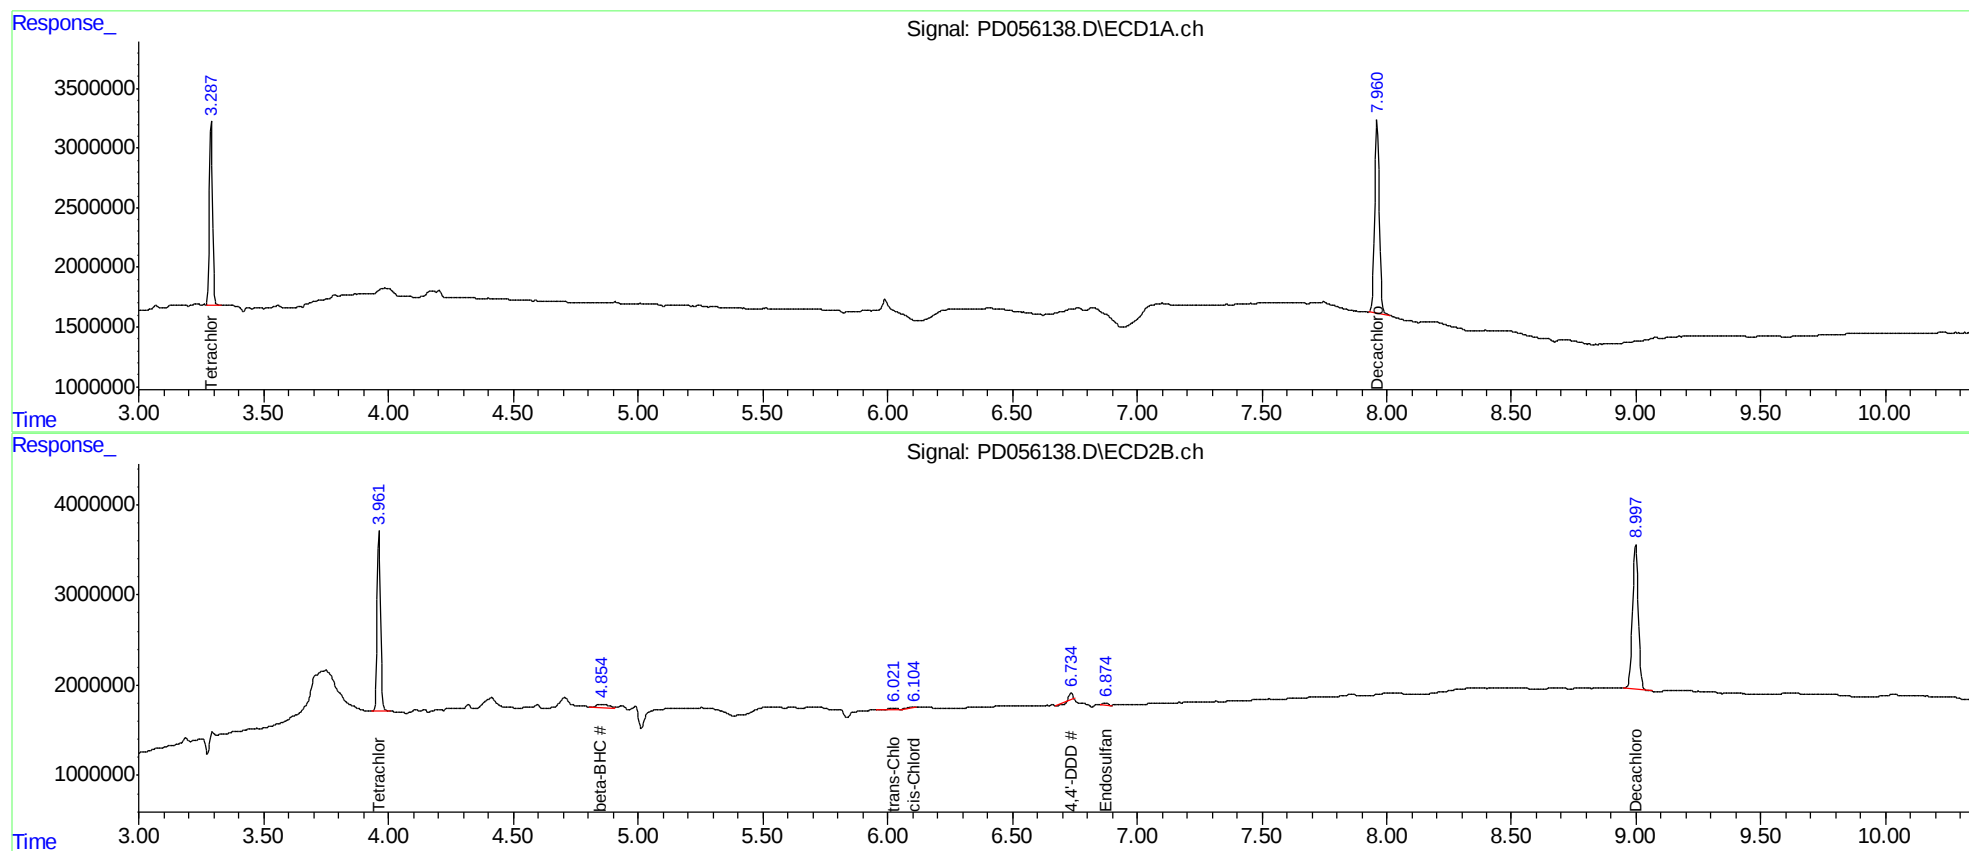


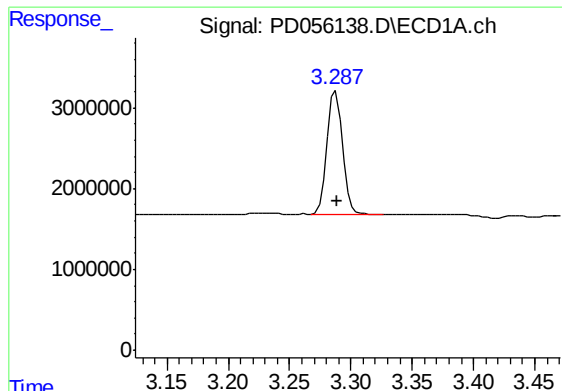

#1 Tetrachloro-m-xylene


R.T.: 3.288 min
Delta R.T.: -0.001 min
Response: 13425103
Conc: 17.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
JLLP2

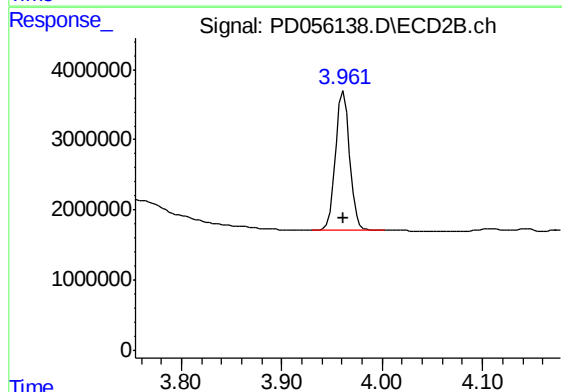


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 19337917
Conc: 18.45 ng/ml

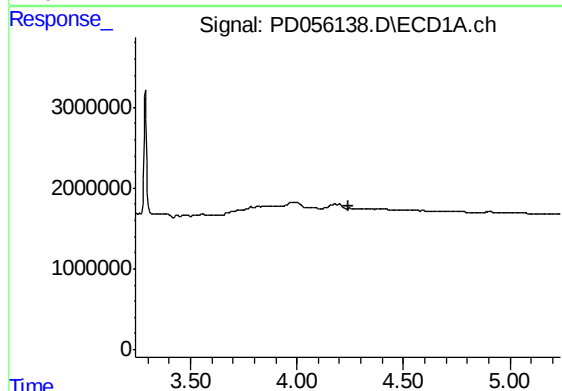


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.240 min
Response: 0
Conc: N.D.

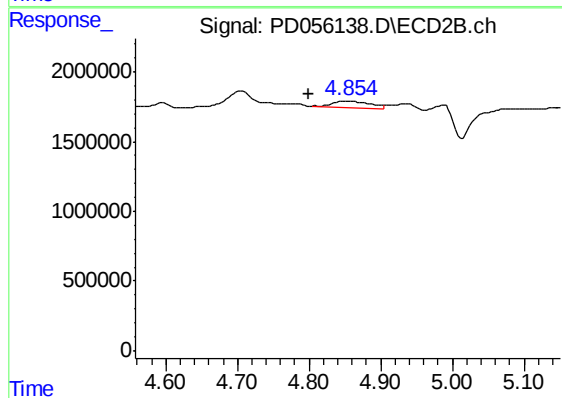

#6 beta-BHC


R.T.: 4.849 min
Delta R.T.: 0.049 min
Response: 1590754
Conc: 2.27 ng/ml

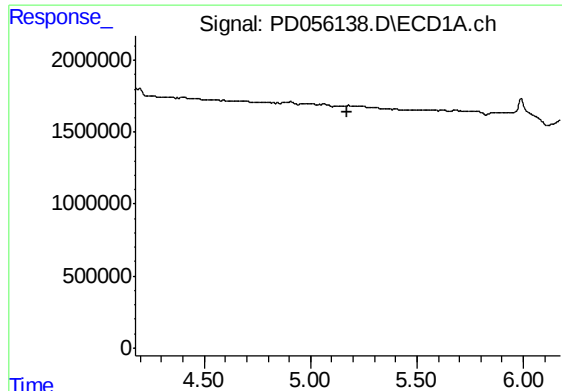

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
JLLP2

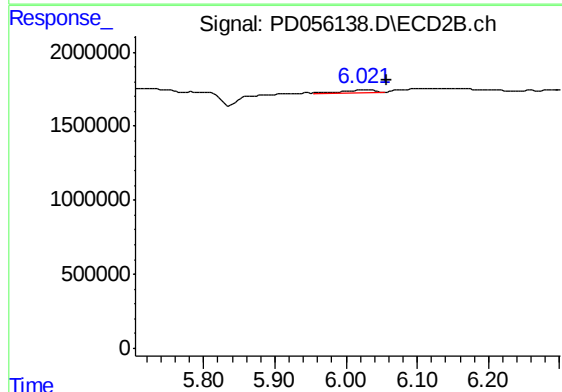


#10 trans-Chlordane

R.T.: 6.023 min
Delta R.T.: -0.035 min
Response: 619416
Conc: 0.43 ng/ml

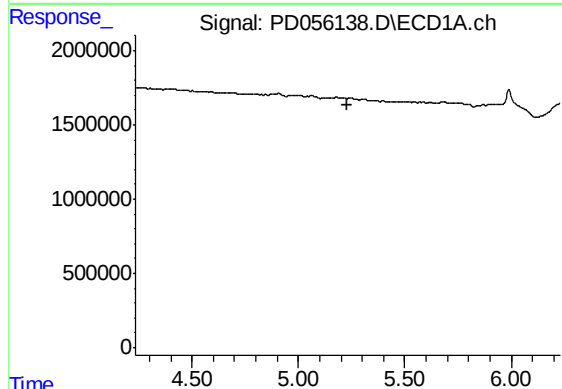


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.231 min
Response: 0
Conc: N.D.

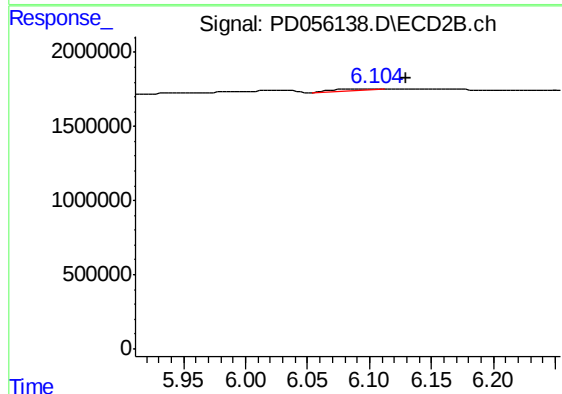

#11 cis-Chlordane


R.T.: 6.105 min
Delta R.T.: -0.025 min
Response: 232578
Conc: 0.17 ng/ml

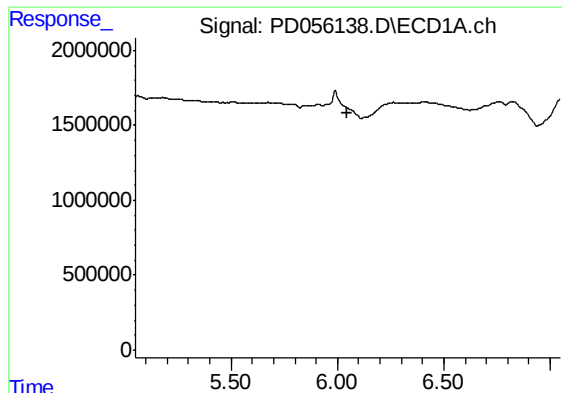

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
JLLP2

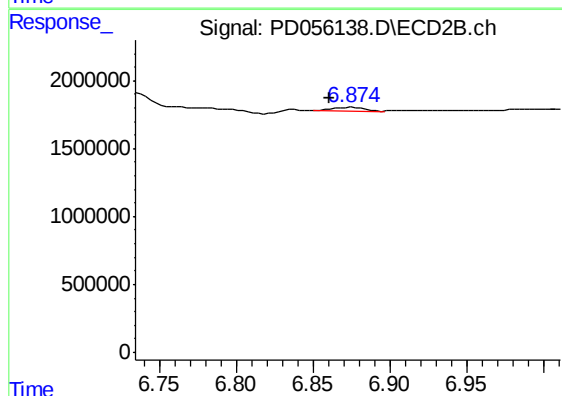


#15 Endosulfan II

R.T.: 6.875 min
Delta R.T.: 0.015 min
Response: 357714
Conc: 0.28 ng/ml

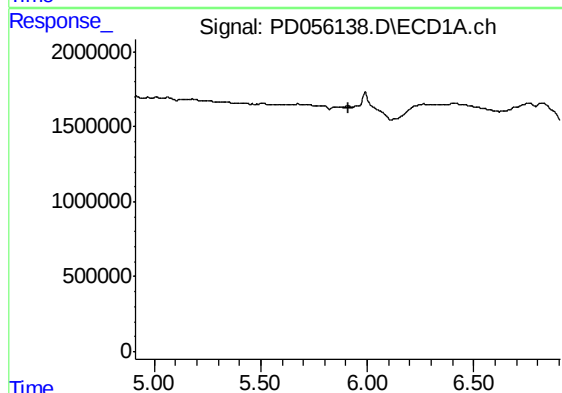


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.911 min
Response: 0
Conc: N.D.

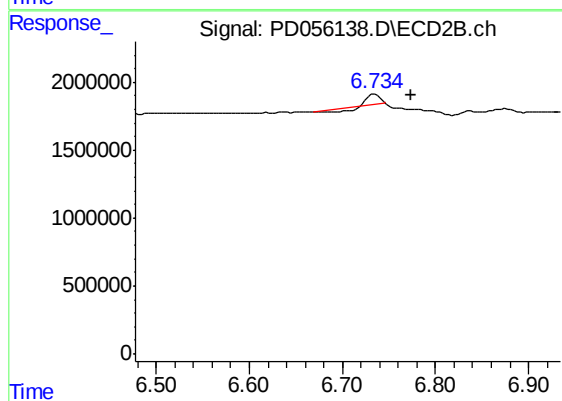

#16 4,4'-DDD


R.T.: 6.735 min
Delta R.T.: -0.039 min
Response: 299168
Conc: 0.27 ng/ml

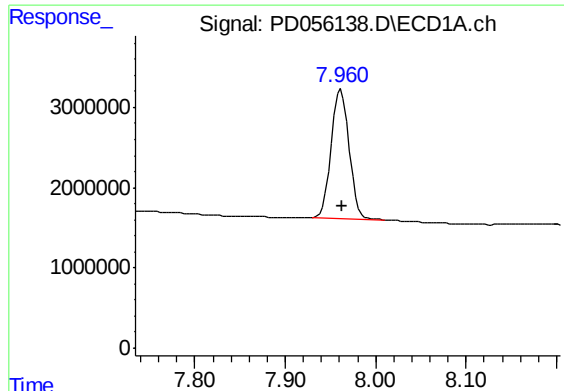

#27 Decachlorobiphenyl

R.T.: 7.962 min
Delta R.T.: -0.001 min
Response: 22200009
Conc: 27.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
JLLP2

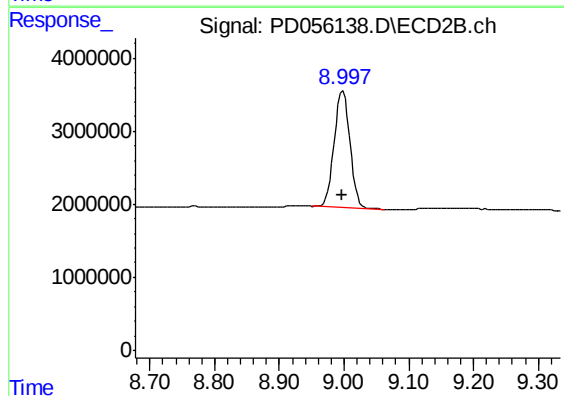

#27 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.001 min
Response: 26780347
Conc: 23.58 ng/ml