

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112019\
 Data File : PD056143.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2019 22:28
 Operator : SG\AJ
 Sample : PIBLK34
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK34

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 01:01:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.962	16793712	23554872	22.309	22.477
27)	SA Decachlor...	7.963	8.998	35853287	43049099	43.986	37.910
Target Compounds							
3)	MA gamma-BHC...	0.000	4.596f	0	53574	N.D.	<MDL
6)	B beta-BHC	0.000	4.847f	0	1037317	N.D.	1.483
8)	B Heptachlo...	0.000	5.819	0	446956	N.D.	0.331
10)	B trans-Chl...	0.000	6.105f	0	4423900	N.D.	3.101
11)	B cis-Chlor...	0.000	6.105	0	4423900	N.D.	3.152
14)	MA Endrin	0.000	6.656	0	787302	N.D.	0.684
16)	A 4,4'-DDD	0.000	6.737f	0	834661	N.D.	0.747
20)	A Methoxychlor	0.000	7.469f	0	101973	N.D.	0.164
23)	Toxaphene-2	0.000	6.656	0	787302	N.D.	65.594


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112019\
Data File : PD056143.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2019 22:28
Operator : SG\AJ
Sample : PIBLK34
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK34

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 01:01:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

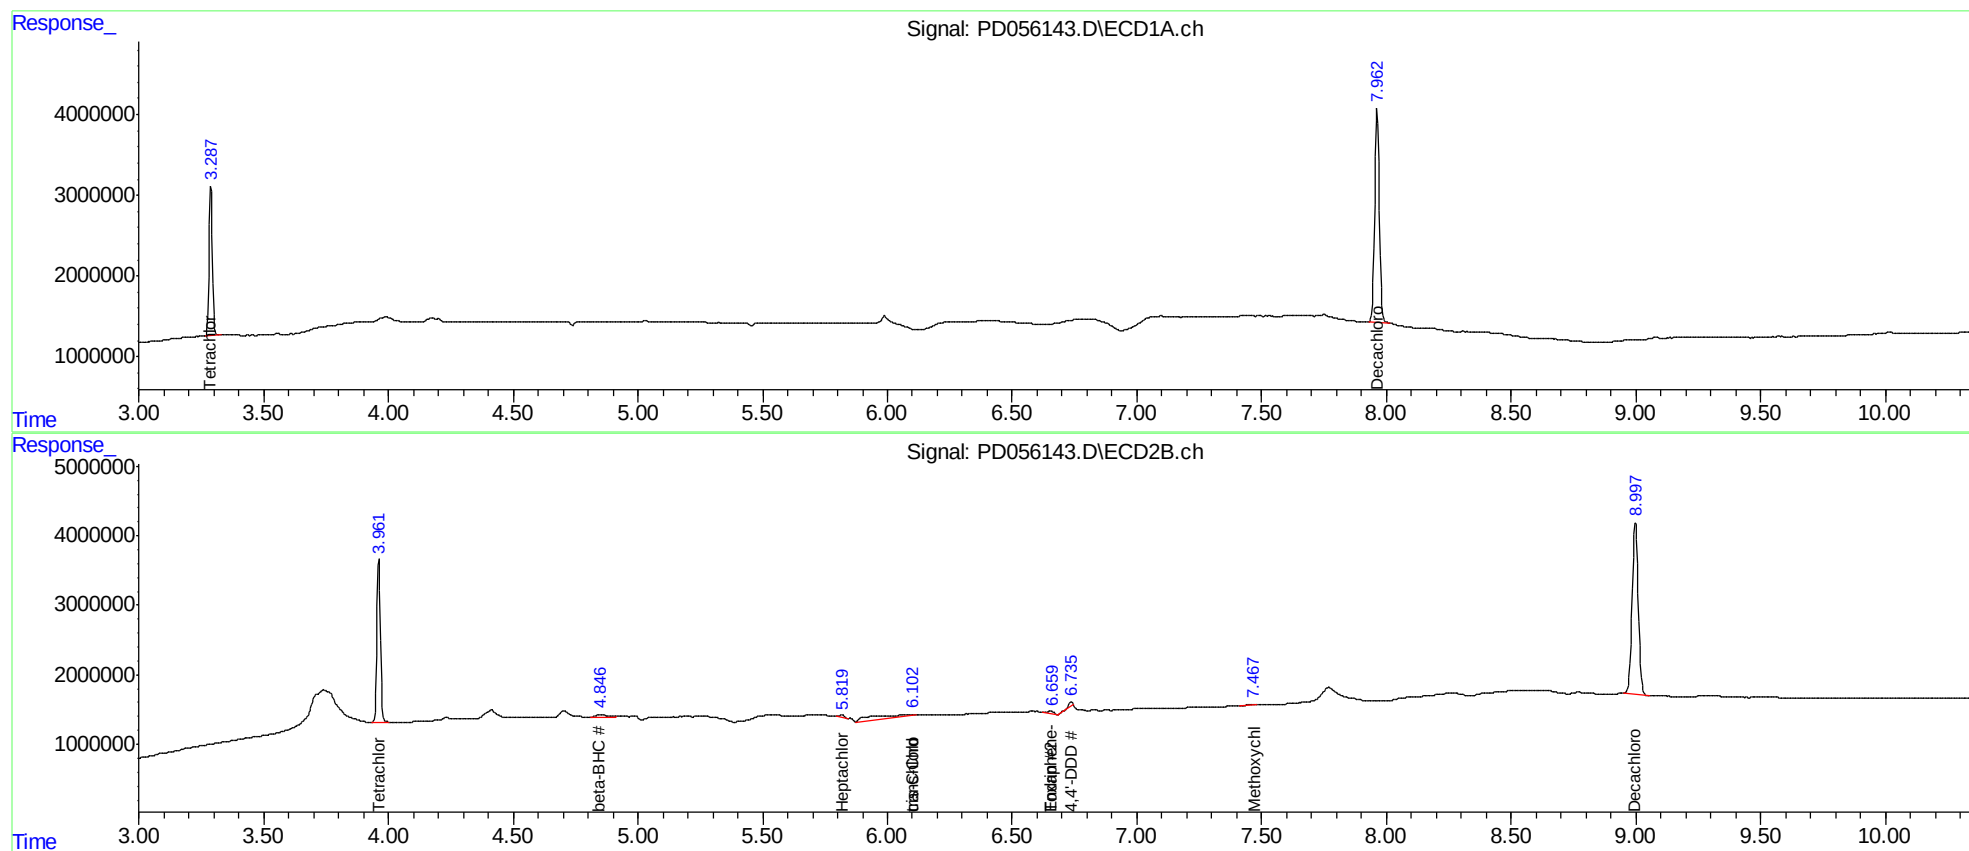


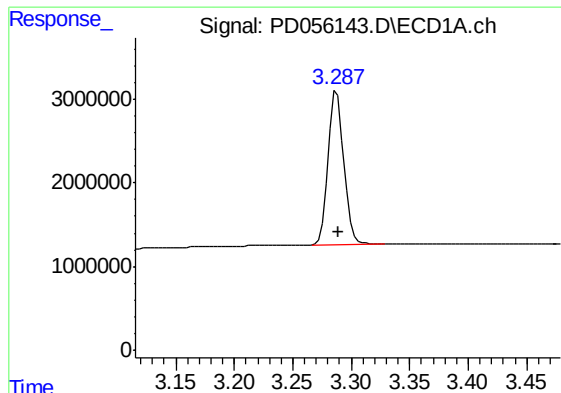

#1 Tetrachloro-m-xylene


R.T.: 3.288 min
Delta R.T.: 0.000 min
Response: 16793712
Conc: 22.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK34

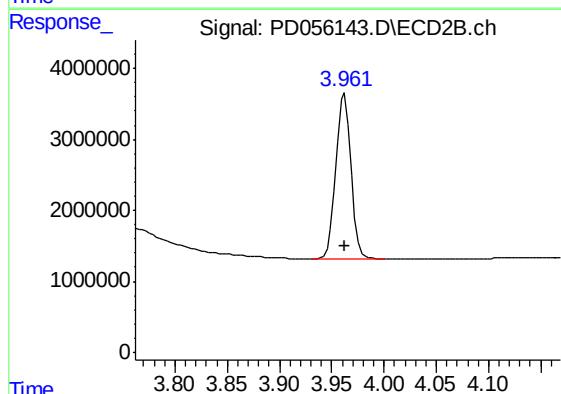


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 23554872
Conc: 22.48 ng/ml

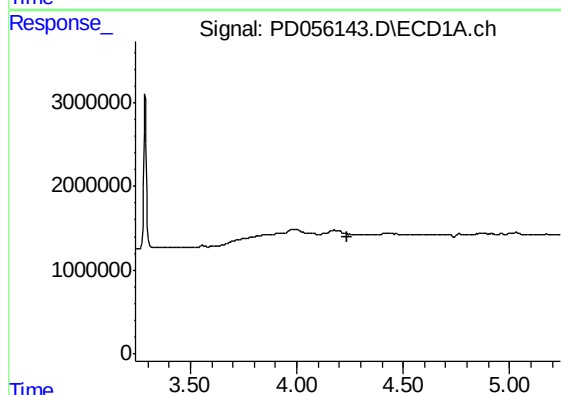


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.240 min
Response: 0
Conc: N.D.

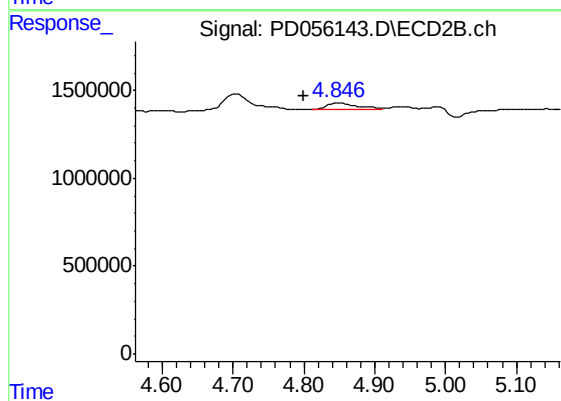

#6 beta-BHC


R.T.: 4.847 min
Delta R.T.: 0.048 min
Response: 1037317
Conc: 1.48 ng/ml

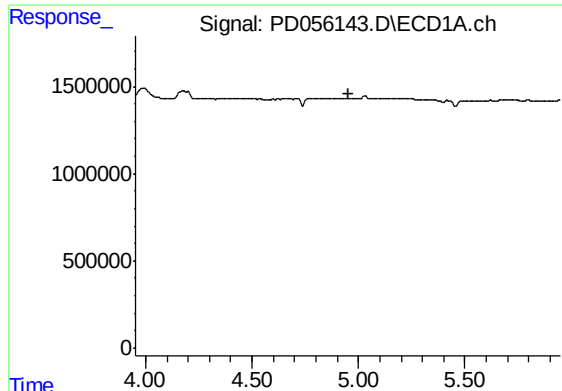

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.952 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK34

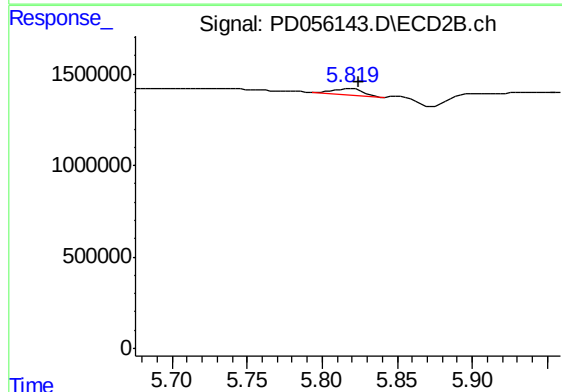


#8 Heptachlor epoxide

R.T.: 5.819 min
Delta R.T.: -0.006 min
Response: 446956
Conc: 0.33 ng/ml

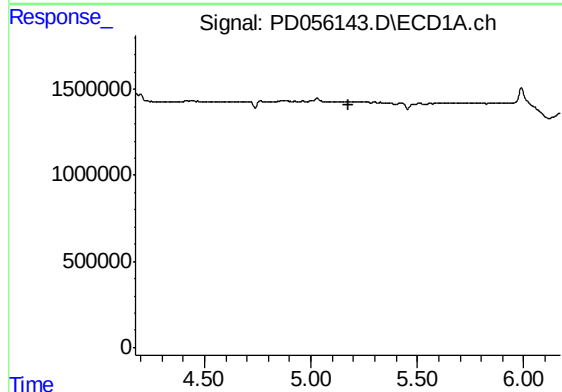


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

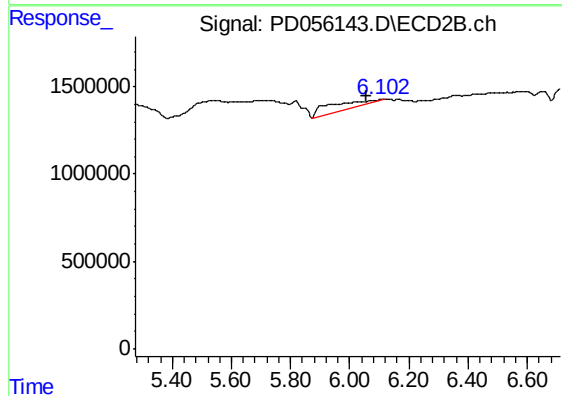

#10 trans-Chlordane


R.T.: 6.105 min
Delta R.T.: 0.047 min
Response: 4423900
Conc: 3.10 ng/ml

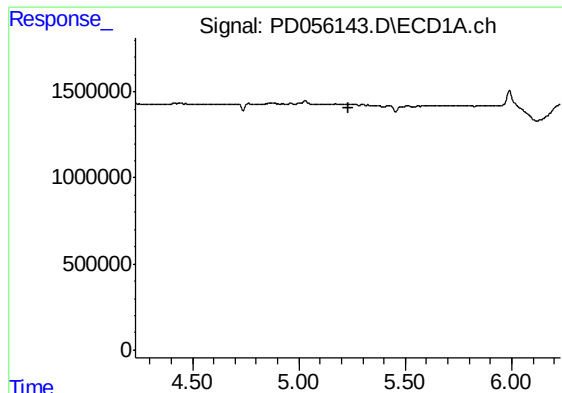

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK34

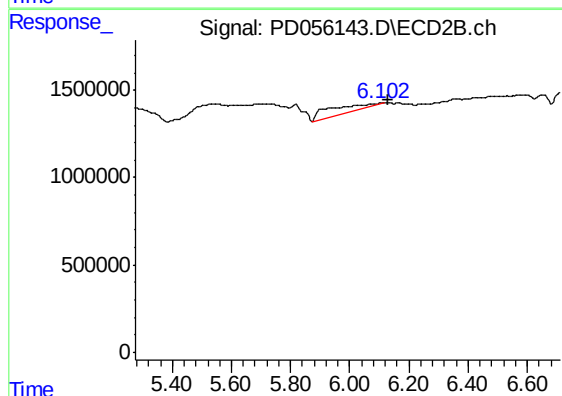


#11 cis-Chlordane

R.T.: 6.105 min
Delta R.T.: -0.025 min
Response: 4423900
Conc: 3.15 ng/ml

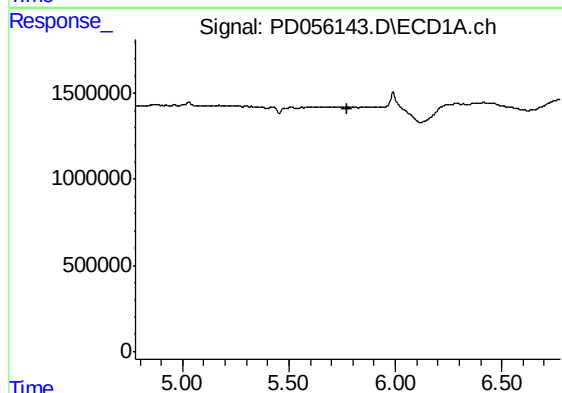


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.776 min
Response: 0
Conc: N.D.

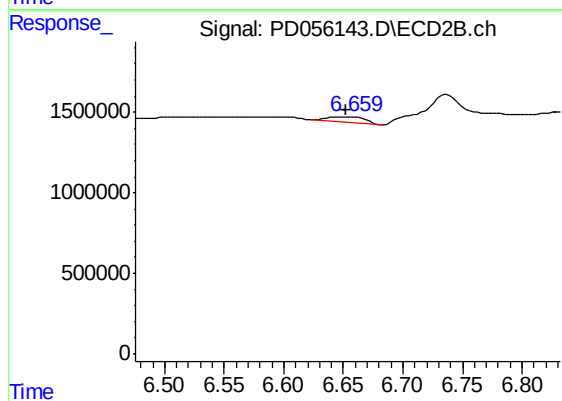

#14 Endrin


R.T.: 6.656 min
Delta R.T.: 0.004 min
Response: 787302
Conc: 0.68 ng/ml

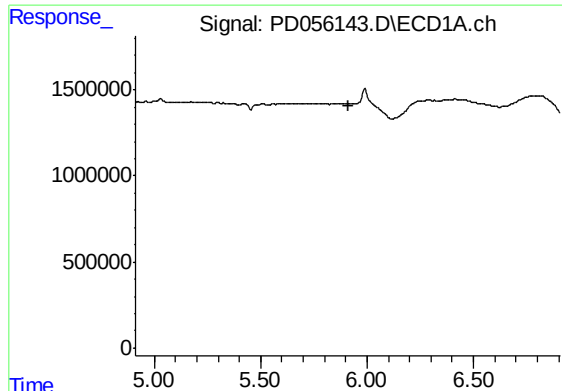

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 5.911 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK34

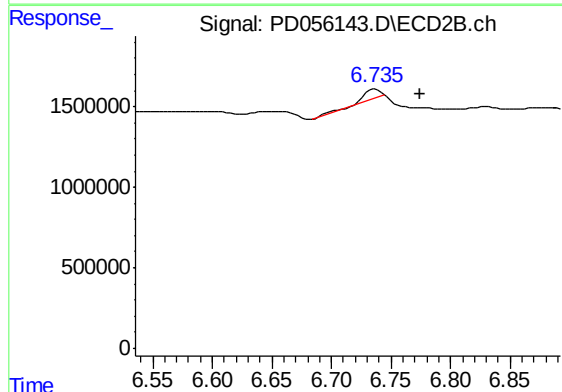


#16 4,4'-DDD

R.T.: 6.737 min
Delta R.T.: -0.037 min
Response: 834661
Conc: 0.75 ng/ml

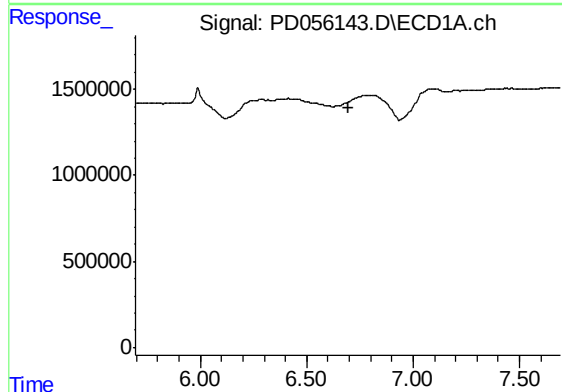


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.695 min
Response: 0
Conc: N.D.

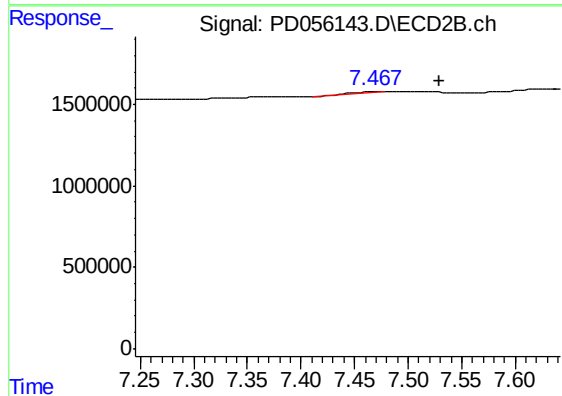

#20 Methoxychlor


R.T.: 7.469 min
Delta R.T.: -0.060 min
Response: 101973
Conc: 0.16 ng/ml

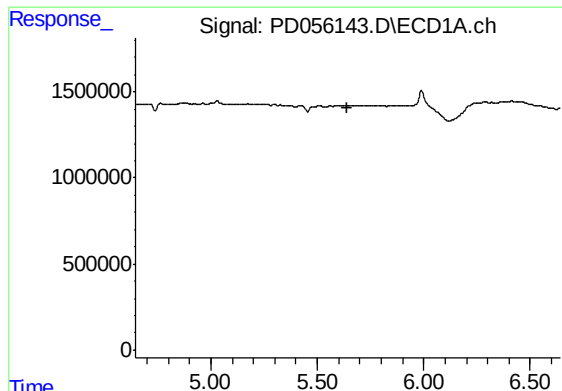

#23 Toxaphene-2


R.T.: 0.000 min
Exp R.T.: 5.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK34

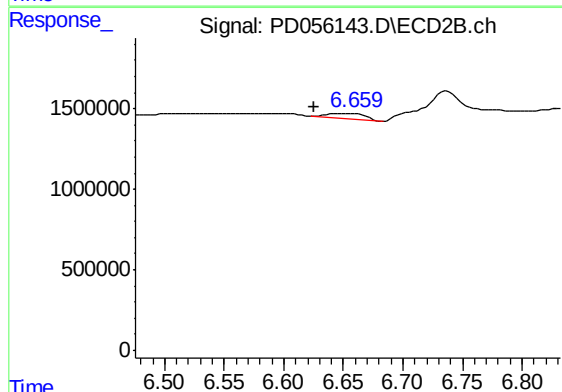


#23 Toxaphene-2

R.T.: 6.656 min
Delta R.T.: 0.031 min
Response: 787302
Conc: 65.59 ng/ml

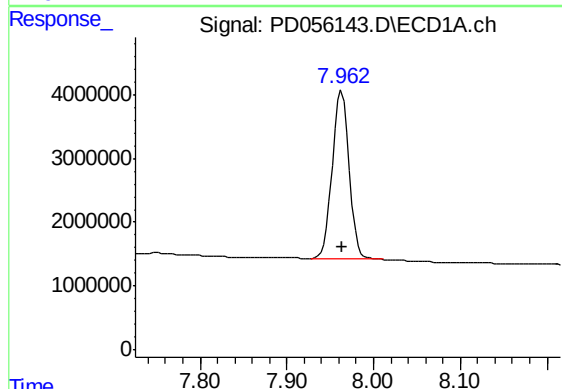

#27 Decachlorobiphenyl

R.T.: 7.963 min
Delta R.T.: 0.000 min
Response: 35853287
Conc: 43.99 ng/ml

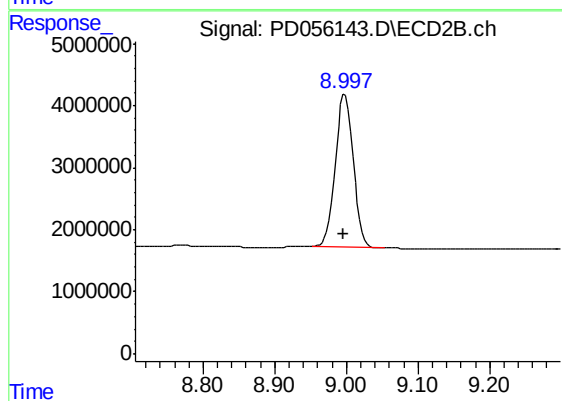

#27 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.001 min
Response: 43049099
Conc: 37.91 ng/ml