

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112019\
 Data File : PD056113.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2019 14:52
 Operator : SG\AJ
 Sample : K5820-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AZ3

Manual Integrations
 APPROVED

Ankita
 11/21/2019 2:01:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 00:53:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.962	17991917	20623518	23.901m	19.680
27)	SA Decachlor...	7.962	8.997	29415287	37308558	36.087	32.855m
Target Compounds							
3)	MA gamma-BHC...	3.996	4.610	7635093	6646140	7.465	4.717m#
14)	MA Endrin	5.775	6.650	1199641	2662438	1.495m	2.313m#
15)	B Endosulfa...	6.050	6.851	1343543	2530924	1.594m	1.954
16)	A 4,4'-DDD	5.913	6.771	6282839	6712620	8.896m	6.011 #
18)	B Endrin al...	6.189	6.979	4972193	3169102	6.960m	2.919m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112019\
Data File : PD056113.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2019 14:52
Operator : SG\AJ
Sample : K5820-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 00:53:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

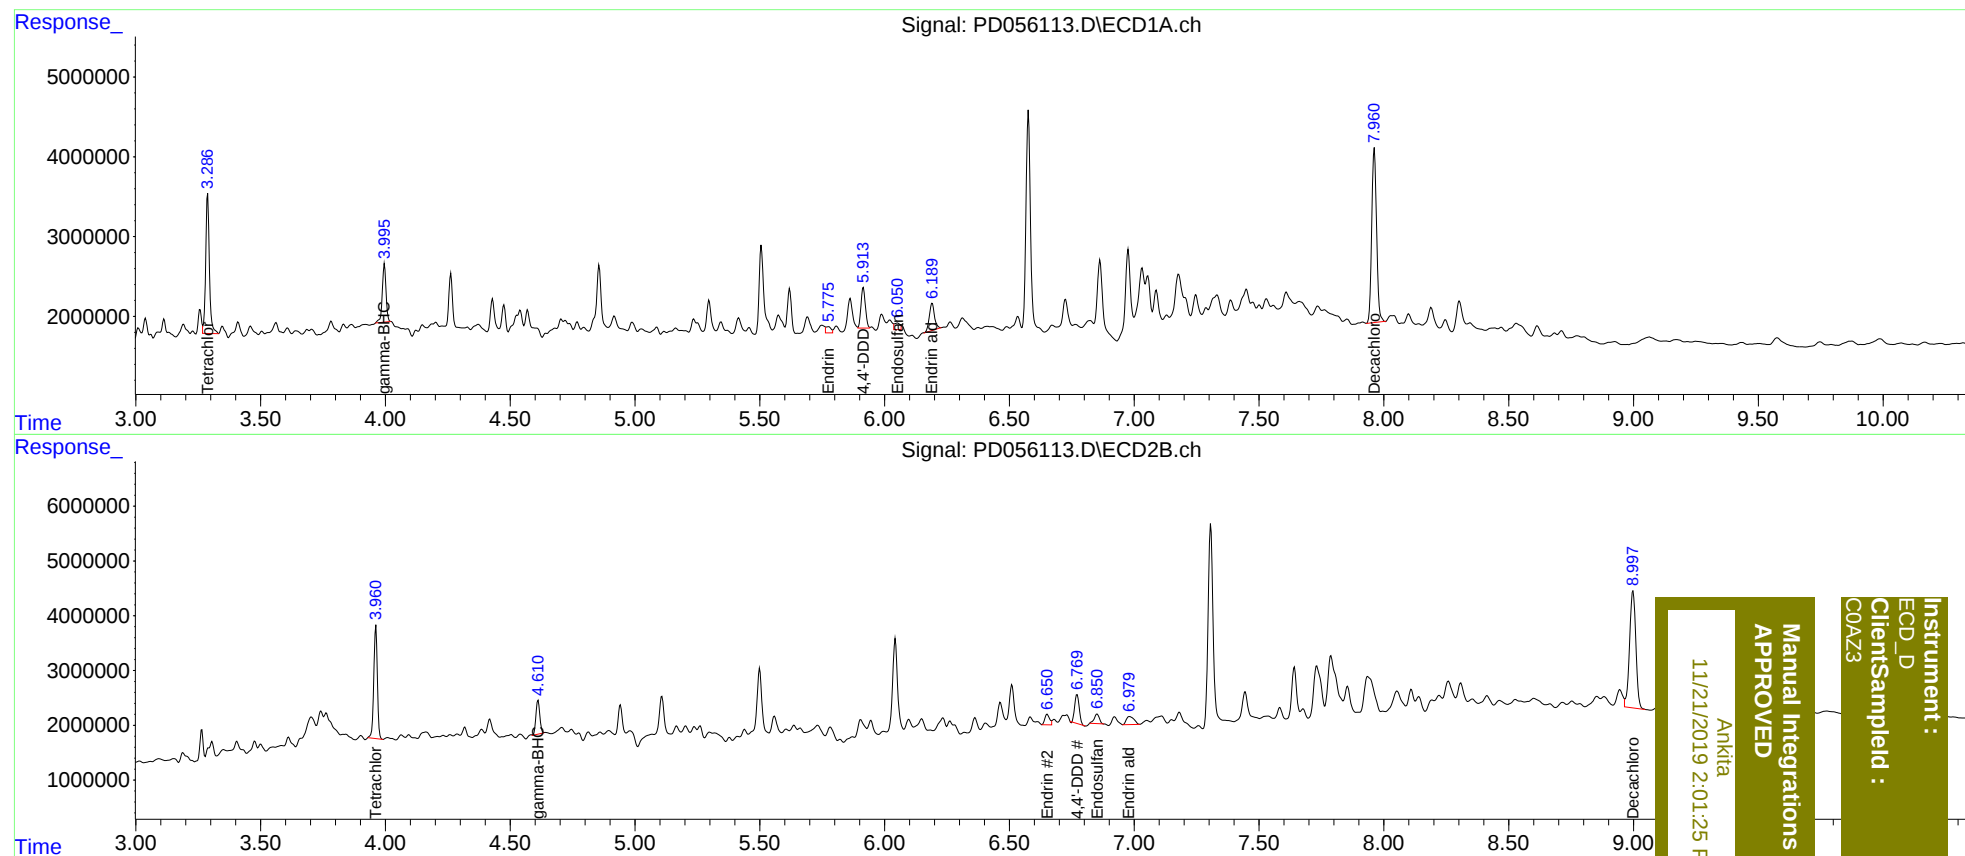

11/21/2019 2:01:25 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client/Sample :
C0A23