

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112020\
 Data File : PD060177.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2020 17:43
 Operator : DD\AJ
 Sample : L4711-13
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0B65

Manual Integrations
 APPROVED

mohammad
 11/23/2020 12:04:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 01:16:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 04:05:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.504	4.023	7746643	27700285	9.040	9.293
2) SA Decachlor...	8.301	9.107	11653723	36924919	14.026	15.010
Target Compounds						
10) B trans-Chl...	5.468	6.137	4882352	35500375	4.597m	10.333m#
11) B cis-Chlor...	5.524	6.212	7823734	90646667	7.396m	26.401m#
12) B 4,4'-DDE	5.688	6.364	5966910	15354645	5.838m	4.749m
17) MA 4,4'-DDT	6.450	7.156	3762617	10848562	4.186m	3.987

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112020\
Data File : PD060177.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2020 17:43
Operator : DD\AJ
Sample : L4711-13
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 01:16:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

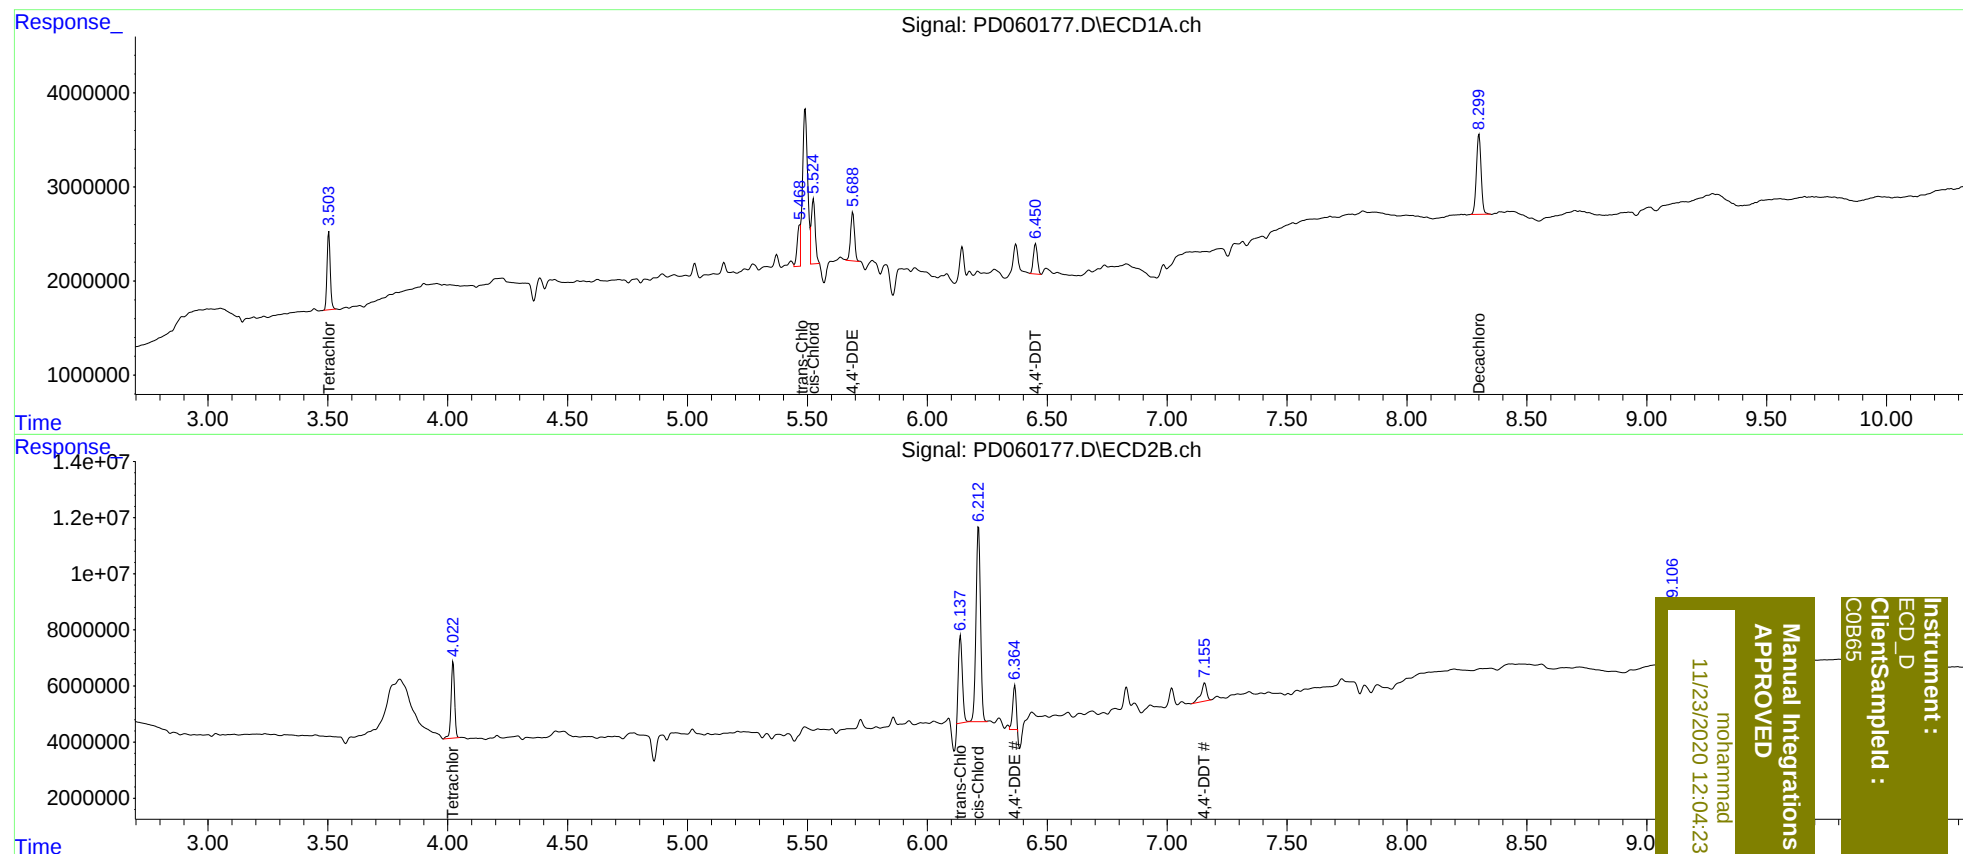

Manual Integrations
APPROVED

mohammad
11/23/2020 12:04:23 PM

Instrument :
ECD_D
ClientSampled :
C0B65