

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112022\
 Data File : PD073144.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2022 16:54
 Operator : AR\AJ
 Sample : N5713-02MS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGC74MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/21/2022
 Supervised By : Ankita Jodhani 11/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 23:41:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.698	3.460	38297443	1375.9E6	15.971	21.063 #
27)	SA Decachlor...	7.827	8.910	56666662	424.2E6	24.833	28.665
Target Compounds							
2)	A alpha-BHC	3.201	3.923	134.7E6	2846.1E6	36.800	32.637
3)	MA gamma-BHC...	3.531	4.256	142.0E6	2625.8E6	42.797	38.700
4)	MA Heptachlor	3.863	4.823	164.9E6	2205.8E6	49.356	48.034
5)	MB Aldrin	4.142	5.161	154.2E6	1774.1E6	45.759	44.175
6)	B beta-BHC	3.833	4.470	62906951	1174.2E6	39.181	43.946m
7)	B delta-BHC	4.062	4.715	11729024	310.4E6	3.227	5.705 #
8)	B Heptachlo...	4.647	5.593	136.6E6	1498.5E6	43.949	44.331
9)	A Endosulfan I	5.016	5.977	125.9E6	1370.3E6	44.535	47.108
10)	B trans-Chl...	4.895	5.846	142.7E6	1398.3E6	46.301	44.264
11)	B cis-Chlor...	4.959	5.922	129.2E6	1428.5E6	41.263	44.998
12)	B 4,4'-DDE	5.147	6.096	290.0E6	2949.8E6	96.945	98.252
13)	MA Dieldrin	5.282	6.254	269.2E6	2897.8E6	87.876	96.134
14)	MA Endrin	5.559	6.487	259.9E6	2366.0E6	95.873	95.918
15)	B Endosulfa...	5.857	6.716	234.4E6	2163.7E6	87.047	89.566
16)	A 4,4'-DDD	5.706	6.621	215.8E6	1819.4E6	89.585	79.385
17)	MA 4,4'-DDT	5.954	6.929	214.7E6	2281.2E6	95.985	106.216
18)	B Endrin al...	6.039	6.847	170.7E6	1528.7E6	79.050	80.696
19)	B Endosulfa...	6.262	7.078	142.3E6	1322.9E6	56.722	63.616m
20)	A Methoxychlor	6.537	7.408	582.3E6	4590.6E6	464.946	492.006
21)	B Endrin ke...	6.772	7.570	266.6E6	2093.6E6	91.315	93.766

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112022\
Data File : PD073144.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2022 16:54
Operator : AR\AJ
Sample : N5713-02MS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 23:41:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD11722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

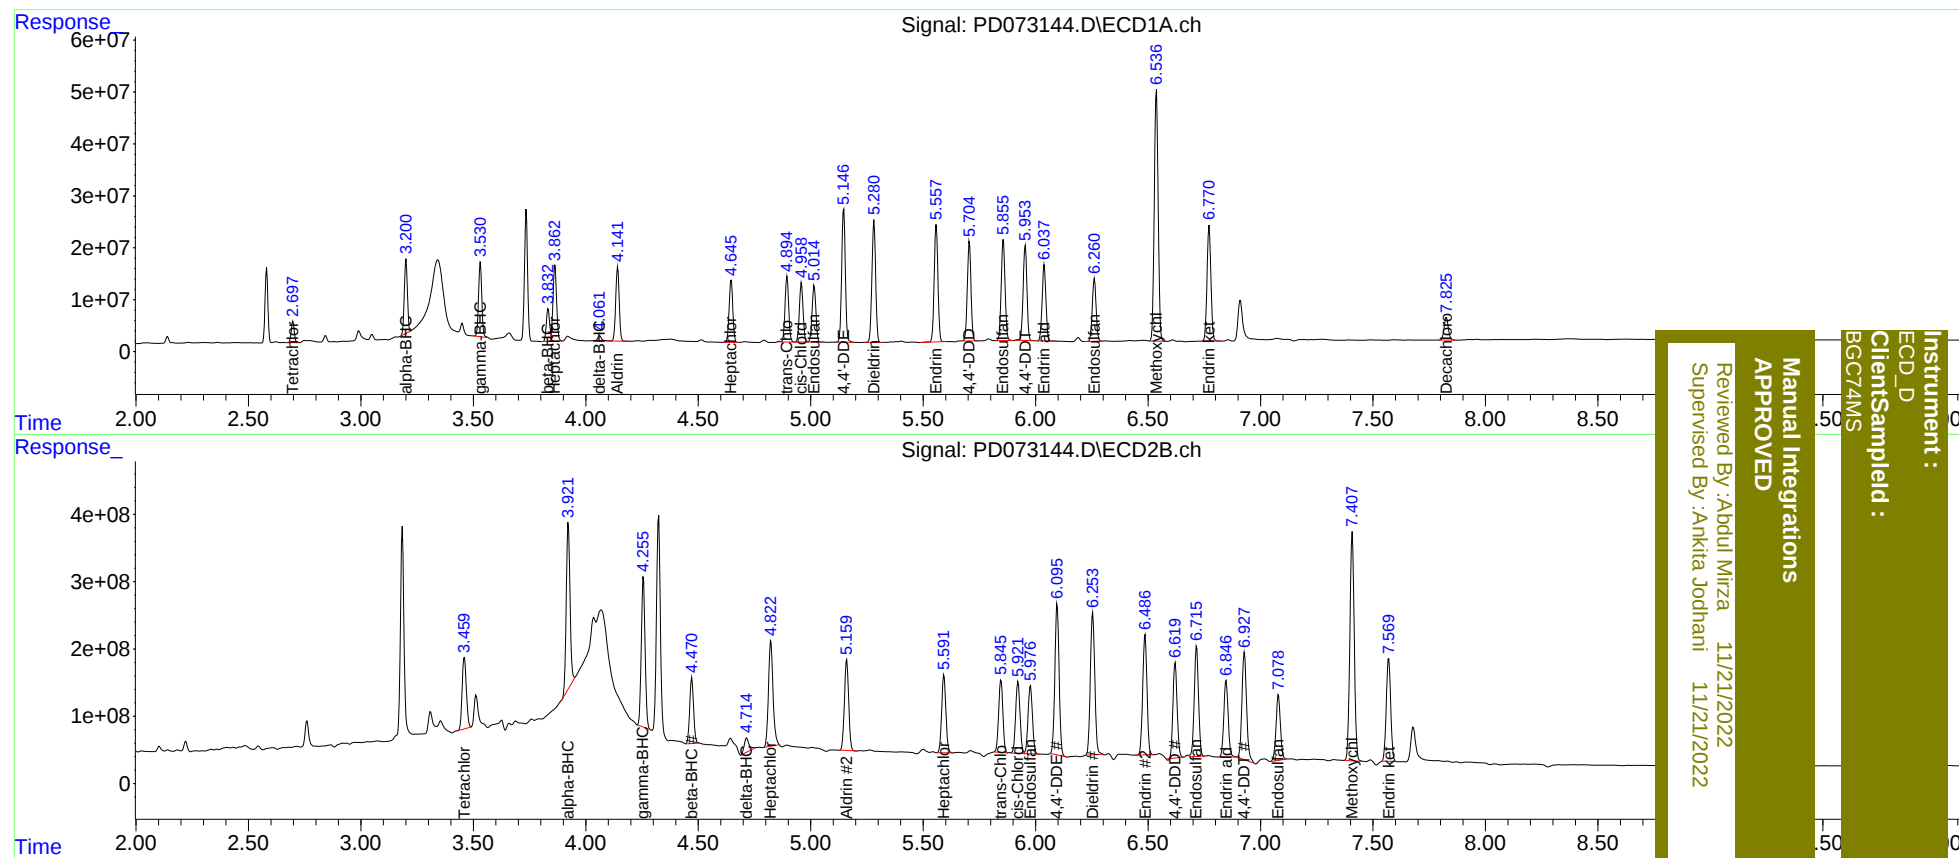

Instrument :
ECD_D
ClientSampled :
BGC74MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 11/21/2022
Supervised By: Ankita Jodhani 11/21/2022