

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112022\
 Data File : PD073145.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2022 17:07
 Operator : AR\AJ
 Sample : N5713-03MSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGC74MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/21/2022
 Supervised By : Ankita Jodhani 11/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 23:41:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.698	3.460	37600465	1384.2E6	15.680	21.190 #
27)	SA Decachlor...	7.826	8.911	56135578	421.5E6	24.601	28.481
Target Compounds							
2)	A alpha-BHC	3.201	3.923	133.6E6	2812.0E6	36.493	32.245
3)	MA gamma-BHC...	3.531	4.256	141.4E6	2619.2E6	42.593	38.602
4)	MA Heptachlor	3.863	4.823	166.6E6	2244.4E6	49.879	48.875
5)	MB Aldrin	4.142	5.161	153.9E6	1774.8E6	45.656	44.193
6)	B beta-BHC	3.832	4.470	62640886	1177.7E6	39.016	44.078m
7)	B delta-BHC	4.062	4.716	11654779	329.5E6	3.207	6.055 #
8)	B Heptachlo...	4.646	5.592	135.4E6	1500.1E6	43.593	44.379
9)	A Endosulfan I	5.016	5.977	125.9E6	1361.1E6	44.542	46.791
10)	B trans-Chl...	4.895	5.846	142.9E6	1395.7E6	46.378	44.180
11)	B cis-Chlor...	4.958	5.922	129.6E6	1433.1E6	41.386	45.142
12)	B 4,4'-DDE	5.146	6.095	289.5E6	2965.3E6	96.770	98.770
13)	MA Dieldrin	5.281	6.254	264.4E6	2930.4E6	86.293	97.217
14)	MA Endrin	5.558	6.486	258.9E6	2322.1E6	95.507	94.138
15)	B Endosulfa...	5.856	6.715	234.0E6	2162.1E6	86.892	89.497
16)	A 4,4'-DDD	5.705	6.620	215.0E6	1818.1E6	89.232	79.331
17)	MA 4,4'-DDT	5.954	6.928	212.7E6	2257.6E6	95.065	105.115
18)	B Endrin al...	6.038	6.847	169.0E6	1522.5E6	78.231	80.366
19)	B Endosulfa...	6.261	7.078	142.1E6	1300.4E6	56.629	62.534m
20)	A Methoxychlor	6.537	7.407	583.9E6	4587.8E6	466.188	491.698
21)	B Endrin ke...	6.772	7.569	266.8E6	2090.5E6	91.413	93.629

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112022\
Data File : PD073145.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2022 17:07
Operator : AR\AJ
Sample : N5713-03MSD
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 23:41:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

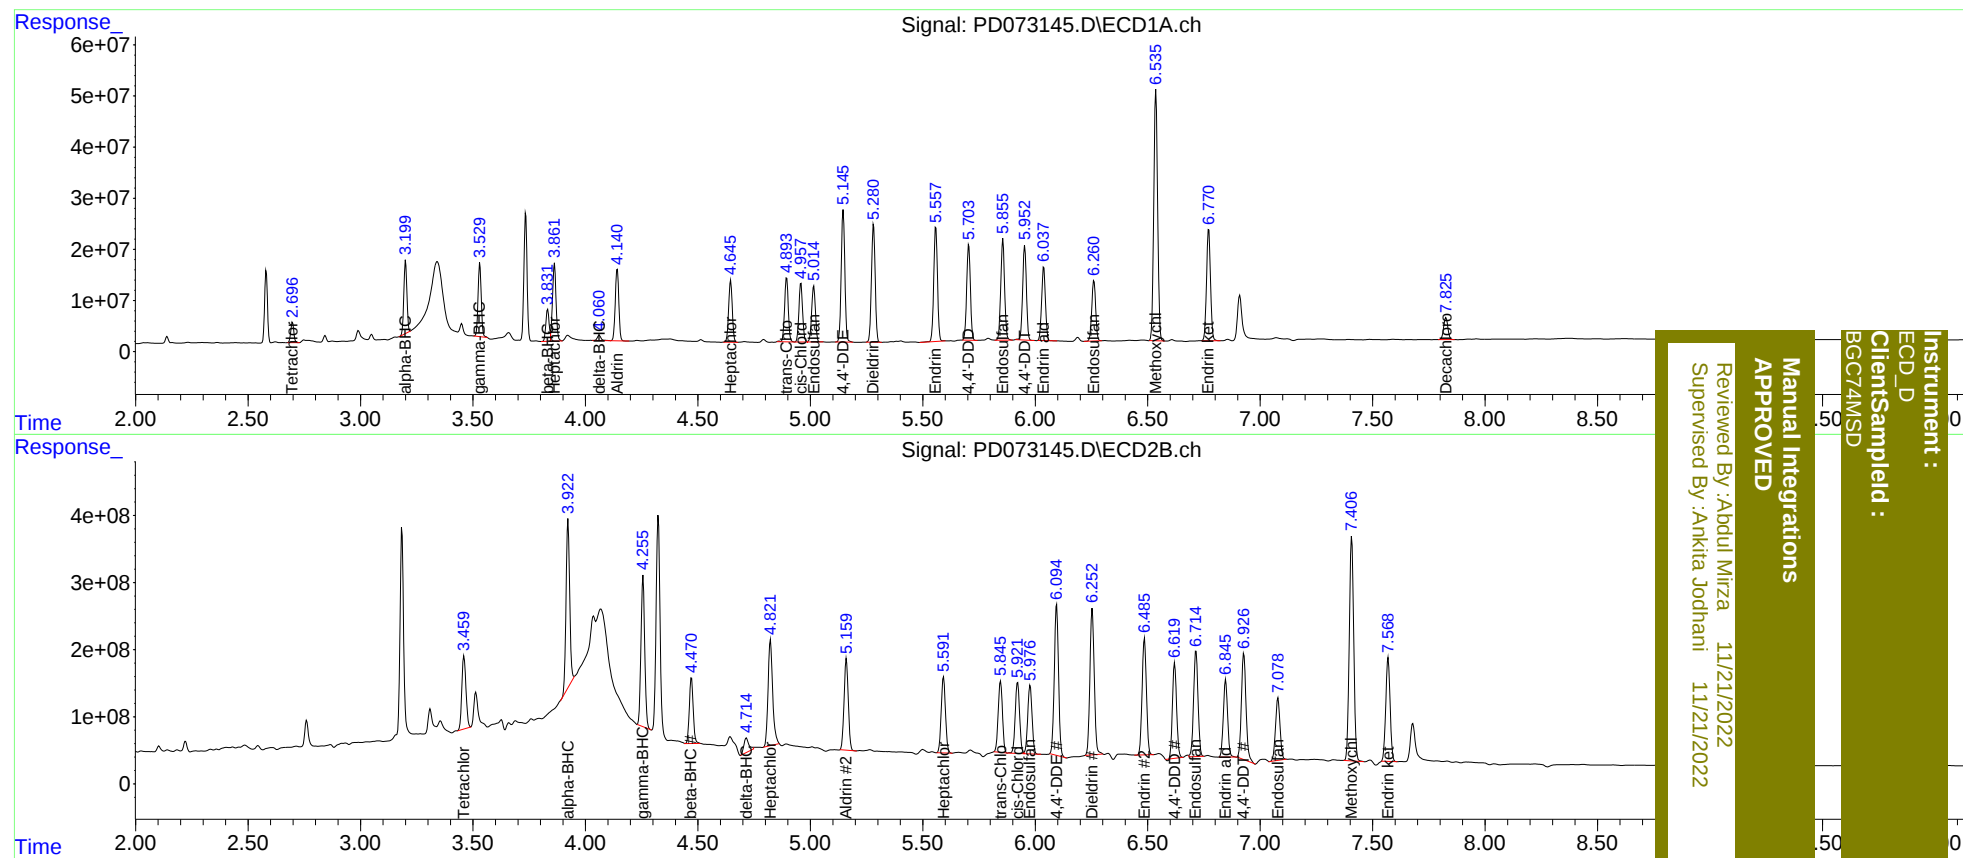

Instrument :
ECD_D
ClientSampled :
BGC74MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 11/21/2022
Supervised By: Ankita Jodhani 11/21/2022