

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112022\
 Data File : PD073142.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2022 16:22
 Operator : AR\AJ
 Sample : PB149179BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS179

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/21/2022
 Supervised By :Ankita Jodhani 11/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 23:40:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.698	3.459	46045317	1301.8E6	19.202	19.929
27)	SA Decachlor...	7.827	8.910	85670584	606.1E6	37.544	40.958
Target Compounds							
2)	A alpha-BHC	3.200	3.922	16452577	475.1E6	4.496	5.448
3)	MA gamma-BHC...	3.530	4.256	15871029	375.7E6	4.782	5.537
4)	MA Heptachlor	3.862	4.822	15868788	257.5E6	4.750	5.608
5)	MB Aldrin	4.141	5.161	16249161	230.0E6	4.822	5.728
6)	B beta-BHC	3.833	4.470	7884296	138.3E6	4.911	5.177m
7)	B delta-BHC	4.062	4.715	15786598	300.1E6	4.344	5.516 #
8)	B Heptachlo...	4.646	5.593	15270015	189.3E6	4.914	5.599
9)	A Endosulfan I	5.015	5.978	14078872	164.7E6	4.982	5.662
10)	B trans-Chl...	4.895	5.847	15318593	176.9E6	4.970	5.601
11)	B cis-Chlor...	4.958	5.922	15177149	174.0E6	4.847	5.482
12)	B 4,4'-DDE	5.146	6.096	26479591	326.4E6	8.851	10.872
13)	MA Dieldrin	5.281	6.254	28804586	336.7E6	9.403	11.171
14)	MA Endrin	5.558	6.486	24508203	262.5E6	9.040	10.641
15)	B Endosulfa...	5.856	6.716	25758995	271.3E6	9.565	11.232
16)	A 4,4'-DDD	5.705	6.620	23058053	267.5E6	9.570	11.673
17)	MA 4,4'-DDT	5.954	6.928	19382594	226.3E6	8.665	10.535
18)	B Endrin al...	6.038	6.847	21476499	216.1E6	9.944	11.406
19)	B Endosulfa...	6.261	7.080	23888625	226.6E6	9.521	10.898
20)	A Methoxychlor	6.537	7.408	59110568	509.8E6	47.195	54.640
21)	B Endrin ke...	6.772	7.570	29680014	263.6E6	10.167	11.804

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112022\
Data File : PD073142.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2022 16:22
Operator : AR\AJ
Sample : PB149179BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 23:40:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

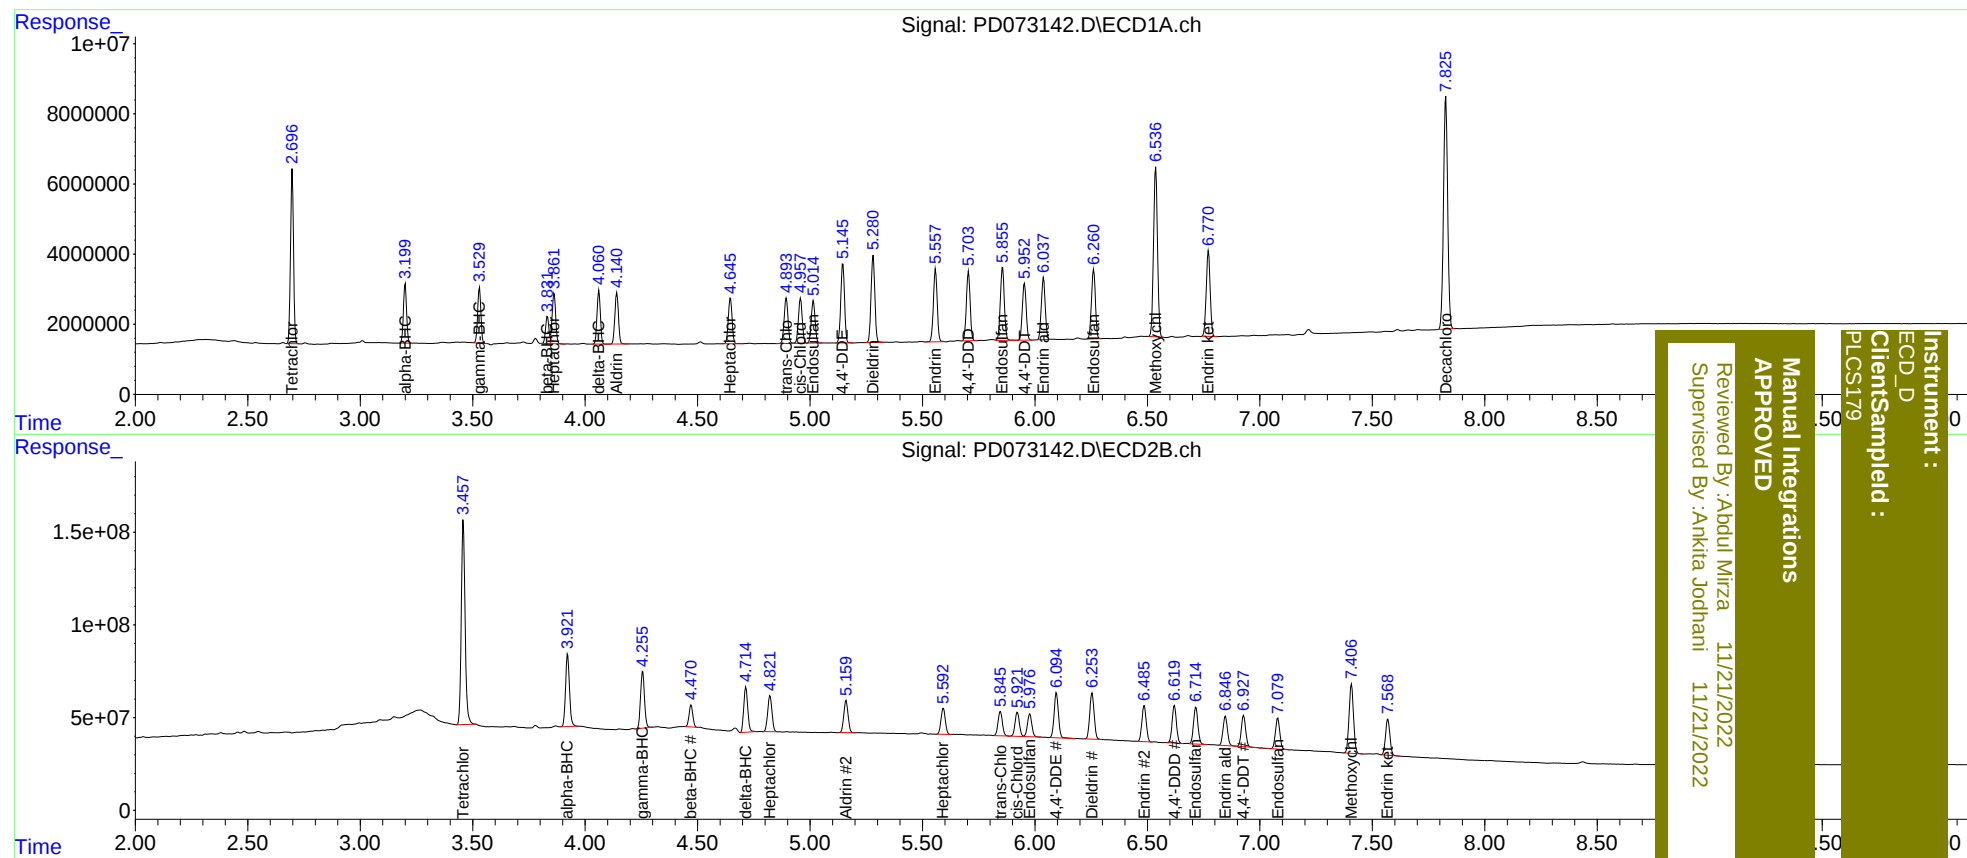

Instrument :
ECD_D
ClientSampled :
PLCS179

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/21/2022
Supervised By :Ankita Jodhani 11/21/2022