

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112023\
 Data File : PD079706.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2023 11:40
 Operator : AR\AJ
 Sample : PB157242BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS242

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/21/2023
 Supervised By :Ankita Jodhani 11/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 20:13:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.802	27791538	43930226	19.030	19.206
27)	SA Decachlor...	9.116	7.947	61573866	79438093	34.698	33.273
Target Compounds							
2)	A alpha-BHC	4.025	3.305	11765344	17654626	4.749	4.869
3)	MA gamma-BHC...	4.359	3.635	11004899	16991739	4.658	4.946
4)	MA Heptachlor	4.952	3.977	13501111	17716481	5.390	5.310
5)	MB Aldrin	5.296	4.258	13002627	18113346	5.545	5.567
6)	B beta-BHC	4.552	3.929	6019118	9230348	5.543	5.636m
7)	B delta-BHC	4.801	4.161	10110012	9697972	4.057	2.714 #
8)	B Heptachlo...	5.722	4.760	12918834	17285449	5.827	5.588
9)	A Endosulfan I	6.109	5.130	12061824	15414478	5.835	5.560
10)	B trans-Chl...	5.978	5.010	12299367	16427335	5.781	5.533
11)	B cis-Chlor...	6.058	5.074	12350754	16491555	5.671	5.433
12)	B 4,4'-DDE	6.228	5.263	21271816	30224015	10.775	10.794
13)	MA Dieldrin	6.384	5.394	23554477	33476846	10.707	10.513
14)	MA Endrin	6.615	5.670	19961644	29494200	10.941	10.769
15)	B Endosulfa...	6.830	5.961	23512942	29214505	12.359m	11.249m
16)	A 4,4'-DDD	6.745	5.817	17134667	25362839	10.577	10.774
17)	MA 4,4'-DDT	7.060	6.069	18480134	24710896	10.847	10.287
18)	B Endrin al...	6.962	6.142	16487161	23054763	11.061	11.393
19)	B Endosulfa...	7.196	6.364	19238344	25319209	10.332	10.190
20)	A Methoxychlor	7.534	6.643	52204895	73288202	56.630	57.017
21)	B Endrin ke...	7.683	6.870	22491619	31708361	11.512	11.153

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112023\
Data File : PD079706.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2023 11:40
Operator : AR\AJ
Sample : PB157242BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 20:13:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

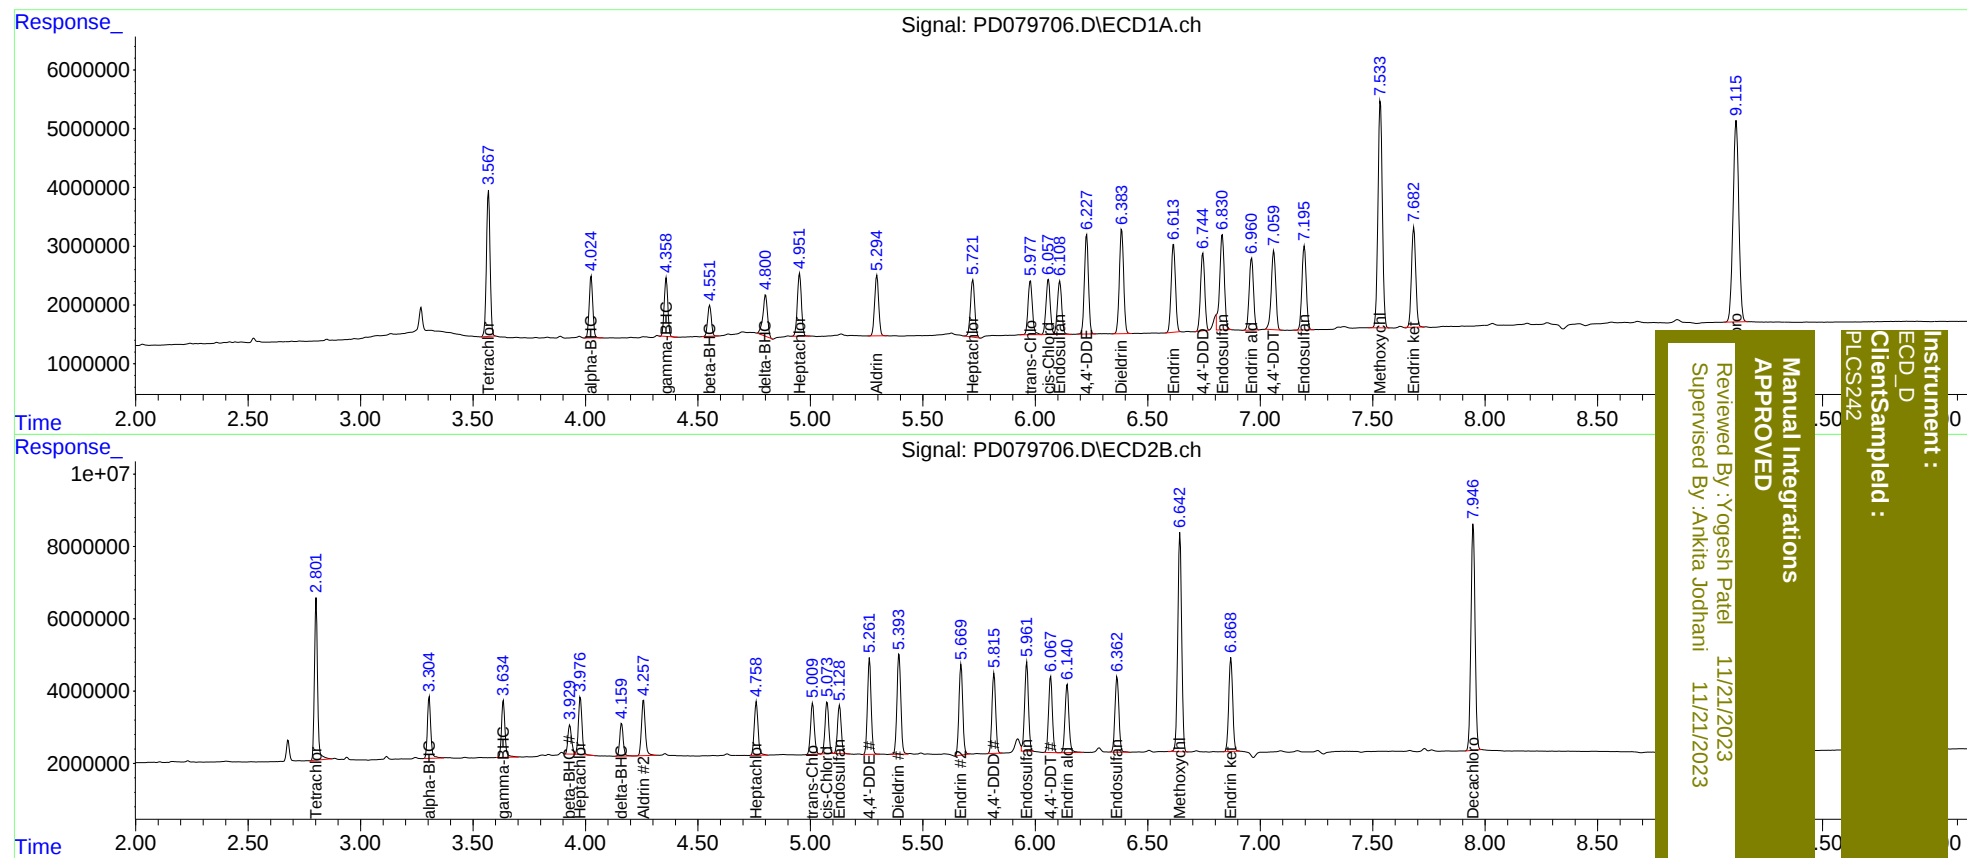

Instrument :
ECD_D
ClientSampled :
PLCS242
Manual Integrations
APPROVED
Reviewed By : Yogesh Patel 11/21/2023
Supervised By : Ankita Jodhani 11/21/2023