

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112023\
 Data File : PD079729.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2023 17:44
 Operator : AR\AJ
 Sample : 05174-20MS
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AN6MS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/21/2023
 Supervised By :Ankita Jodhani 11/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 20:26:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.803	19564405	34407404	13.397	15.043
27)	SA Decachlor...	9.108	7.944	67509398	83740445	38.043m	35.075
Target Compounds							
2)	A alpha-BHC	4.024	3.306	102.6E6	160.7E6	41.410m	44.317
3)	MA gamma-BHC...	4.357	3.636	98252255	162.4E6	41.586m	47.275
4)	MA Heptachlor	4.950	3.978	99587706	139.7E6	39.761m	41.884
5)	MB Aldrin	5.295	4.257	92643345	132.5E6	39.507	40.710m
6)	B beta-BHC	4.553	3.930	32767757	56739823	30.178	34.647
7)	B delta-BHC	4.801	4.162	95735579	155.2E6	38.418	43.428
8)	B Heptachlo...	5.720	4.760	80906535	128.3E6	36.495	41.493
9)	A Endosulfan I	6.107	5.132	76884929	74966642	37.193	27.042 #
10)	B trans-Chl...	5.975	5.010	75007865	126.3E6	35.253m	42.554
11)	B cis-Chlor...	6.056	5.075	85014767	126.4E6	39.034	41.649
12)	B 4,4'-DDE	6.226	5.264	125.5E6	247.3E6	63.573	88.323 #
13)	MA Dieldrin	6.383	5.395	166.3E6	262.2E6	75.595	82.341
14)	MA Endrin	6.613	5.670	135.7E6	227.8E6	74.374	83.187
15)	B Endosulfa...	6.830	5.962	137.7E6	214.4E6	72.401	82.558
16)	A 4,4'-DDD	6.744	5.816	127.6E6	188.9E6	78.759	80.248
17)	MA 4,4'-DDT	7.058	6.067	127.3E6	189.3E6	74.736	78.813
18)	B Endrin al...	6.960	6.140	78597330	112.5E6	52.732	55.601m
19)	B Endosulfa...	7.194	6.363	128.3E6	195.1E6	68.927	78.506
20)	A Methoxychlor	7.532	6.641	338.2E6	459.0E6	366.904	357.104m
21)	B Endrin ke...	7.681	6.869	133.4E6	186.0E6	68.270	65.420

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112023\
Data File : PD079729.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2023 17:44
Operator : AR\AJ
Sample : 05174-20MS
Misc :
ALS Vial : 37 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 20:26:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

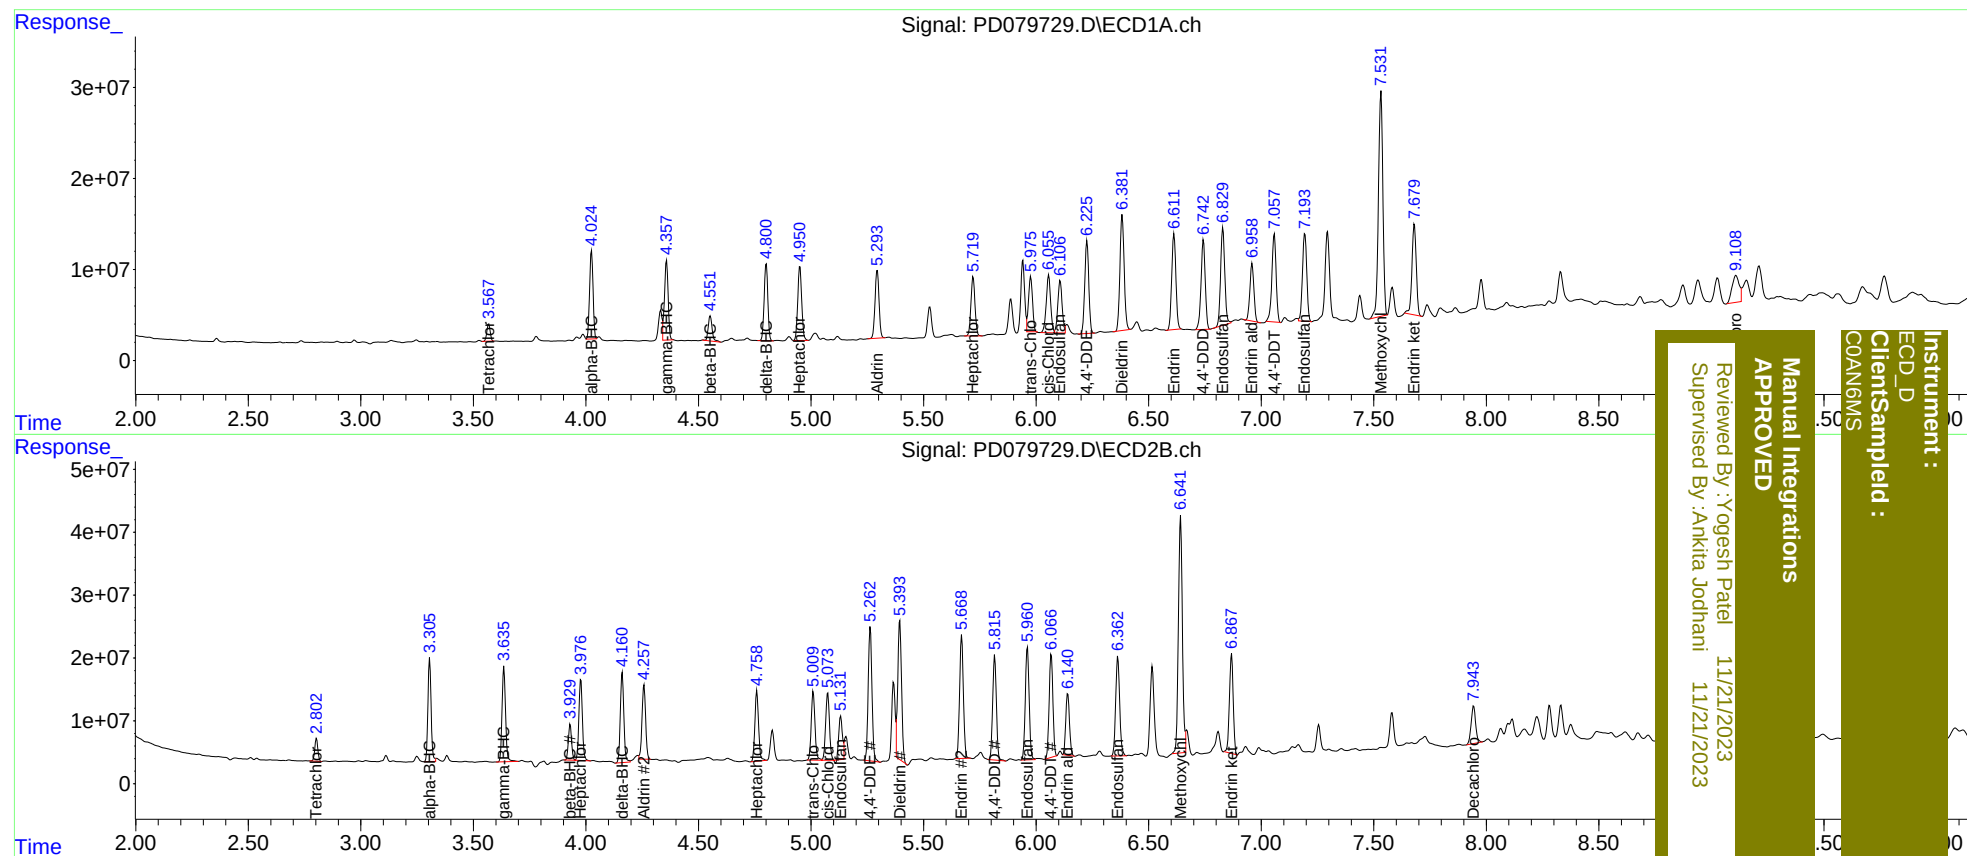

Manual Integrations
APPROVED
Reviewed By : Yogesh Patel 11/21/2023
Supervised By : Ankita Jodhani 11/21/2023

Instrument :
ECD_D
Client Sampled :
COAN6MS