

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112023\
 Data File : PD079730.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2023 18:11
 Operator : AR\AJ
 Sample : 05174-21MSD
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AN6MSD

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/21/2023
 Supervised By :Ankita Jodhani 11/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 20:26:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.568	2.803	19729905	33846597	13.510	14.798
27)	SA Decachlor...	9.106	7.945	71234012	61969710	40.142m	25.956 #
Target Compounds							
2)	A alpha-BHC	4.024	3.306	103.5E6	163.6E6	41.774m	45.125
3)	MA gamma-BHC...	4.357	3.636	96639242	162.7E6	40.903m	47.369
4)	MA Heptachlor	4.951	3.978	96409524	144.4E6	38.492	43.276
5)	MB Aldrin	5.294	4.257	92834820	132.4E6	39.589	40.678m
6)	B beta-BHC	4.553	3.930	32186675	60561857	29.643	36.981
7)	B delta-BHC	4.802	4.162	93898396	157.0E6	37.681	43.943
8)	B Heptachlo...	5.720	4.760	82431304	128.3E6	37.183	41.494
9)	A Endosulfan I	6.107	5.131	77153834	86999827	37.323	31.382m
10)	B trans-Chl...	5.975	5.010	78754282	124.2E6	37.014m	41.843
11)	B cis-Chlor...	6.056	5.075	85485345	123.1E6	39.250	40.553
12)	B 4,4'-DDE	6.226	5.264	122.1E6	242.7E6	61.840	86.668 #
13)	MA Dieldrin	6.383	5.395	167.2E6	263.6E6	76.020	82.797
14)	MA Endrin	6.613	5.670	134.1E6	229.3E6	73.472	83.717
15)	B Endosulfa...	6.831	5.962	137.5E6	212.2E6	72.281	81.704
16)	A 4,4'-DDD	6.743	5.816	127.4E6	188.9E6	78.649	80.232
17)	MA 4,4'-DDT	7.059	6.068	128.0E6	187.3E6	75.117	77.991
18)	B Endrin al...	6.960	6.140	80880086	112.2E6	54.263	55.428m
19)	B Endosulfa...	7.194	6.364	130.8E6	189.8E6	70.222	76.374
20)	A Methoxychlor	7.532	6.643	335.5E6	476.1E6	363.910	370.394
21)	B Endrin ke...	7.681	6.869	130.9E6	185.2E6	67.023	65.142

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112023\
Data File : PD079730.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2023 18:11
Operator : AR\AJ
Sample : 05174-21MSD
Misc :
ALS Vial : 38 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 20:26:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

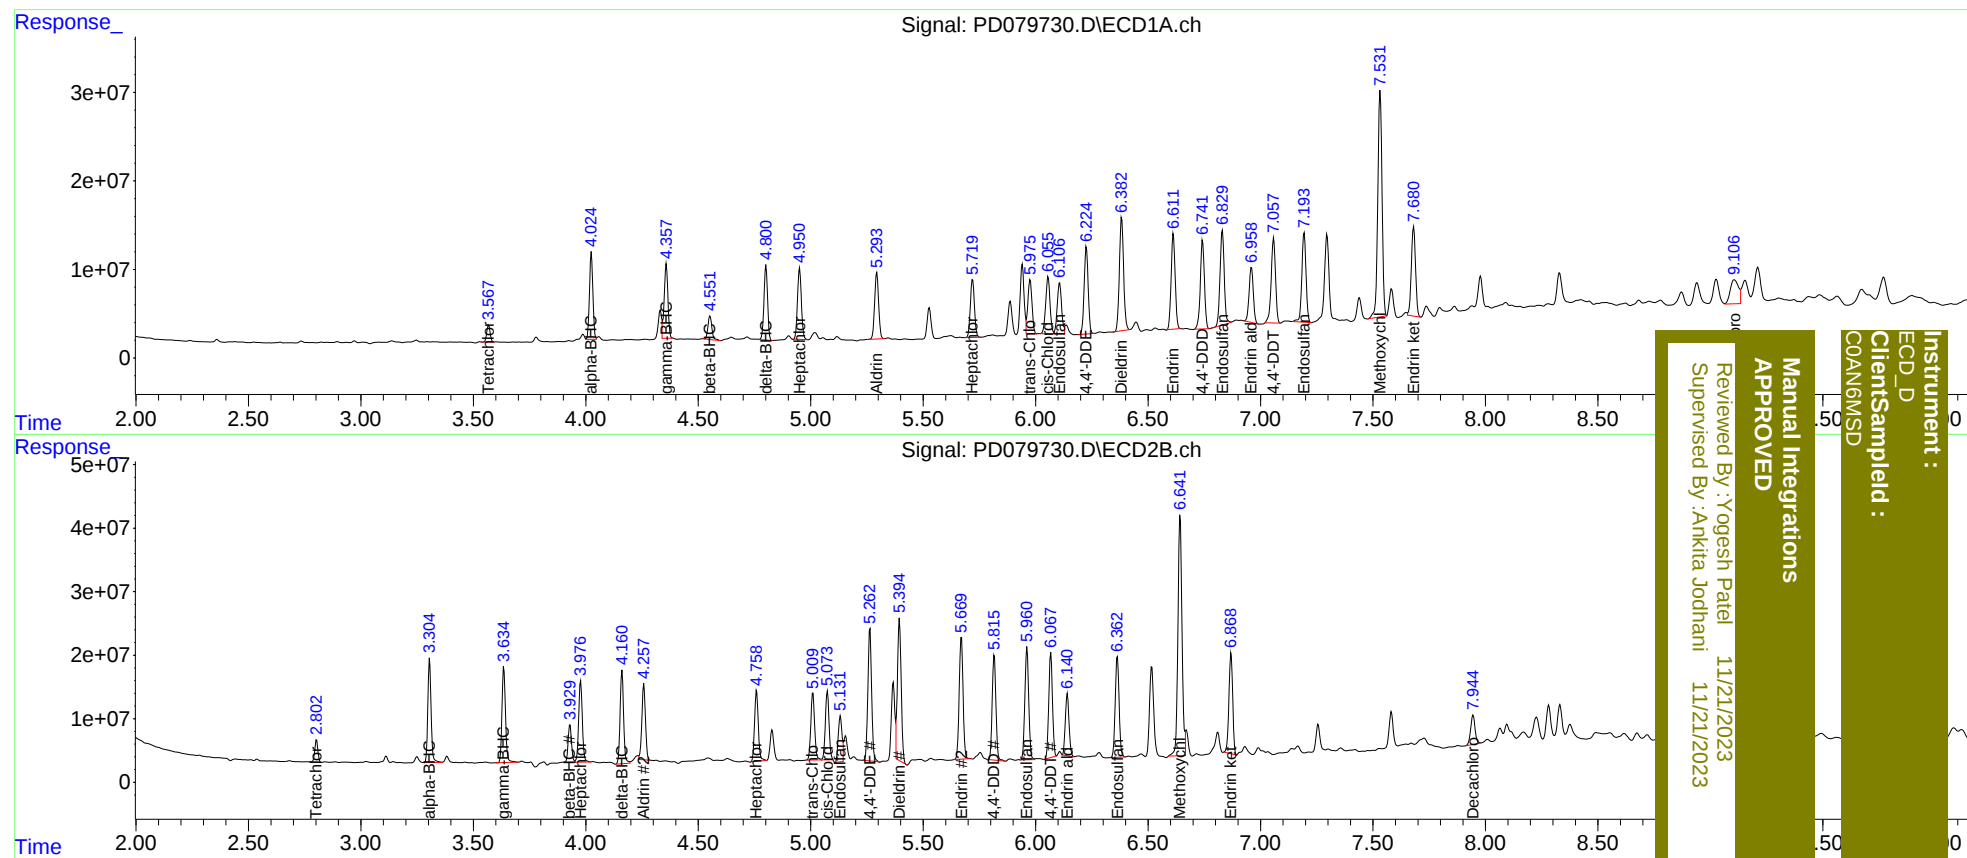

Manual Integrations
APPROVED
Reviewed By : Yogesh Patel 11/21/2023
Supervised By : Ankita Jodhani 11/21/2023

Instrument :
ECD_D
Client Sampled :
COAN6MSD