

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112023\
 Data File : PD079739.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2023 20:38
 Operator : AR\AJ
 Sample : 05390-05MS
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0TJ7MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 04:52:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.568	2.803	25790271	41307048	17.660	18.059
2)	SA Decachlor...	9.111	7.946	31226639	47267703	17.597	19.798
Target Compounds							
2)	A alpha-BHC	4.025	3.306	115.3E6	176.1E6	46.526	48.573
3)	MA gamma-BHC...	4.358	3.635	105.4E6	159.8E6	44.605	46.519
4)	MA Heptachlor	4.951	3.977	105.8E6	155.1E6	42.231	46.503
5)	MB Aldrin	5.295	4.258	99964155	151.2E6	42.629	46.461
6)	B beta-BHC	4.552	3.930	45005709	67854849	41.449	41.434
7)	B delta-BHC	4.801	4.161	107.4E6	165.5E6	43.090	46.317
8)	B Heptachlo...	5.720	4.759	91058128	144.1E6	41.074	46.587
9)	A Endosulfan I	6.107	5.130	85808016	130.5E6	41.509	47.065
10)	B trans-Chl...	5.976	5.010	87591404	139.9E6	41.167	47.126
11)	B cis-Chlor...	6.056	5.074	89662020	139.3E6	41.168	45.897
12)	B 4,4'-DDE	6.227	5.263	171.9E6	277.8E6	87.090	99.195
13)	MA Dieldrin	6.382	5.394	191.0E6	300.8E6	86.837	94.480
14)	MA Endrin	6.613	5.669	162.0E6	259.2E6	88.808	94.647
15)	B Endosulfa...	6.830	5.961	167.3E6	249.8E6	87.961	96.181
16)	A 4,4'-DDD	6.743	5.816	145.9E6	226.8E6	90.089	96.344
17)	MA 4,4'-DDT	7.058	6.068	153.7E6	229.8E6	90.199	95.657
18)	B Endrin al...	6.960	6.140	121.6E6	181.0E6	81.613	89.435
19)	B Endosulfa...	7.194	6.363	157.3E6	232.2E6	84.490	93.460
20)	A Methoxychlor	7.532	6.642	386.2E6	561.7E6	418.929	436.956
21)	B Endrin ke...	7.681	6.869	165.5E6	265.2E6	84.702	93.288

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD11023\
Data File : PD079739.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2023 20:38
Operator : AR\AJ
Sample : 05390-05MS
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 04:52:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

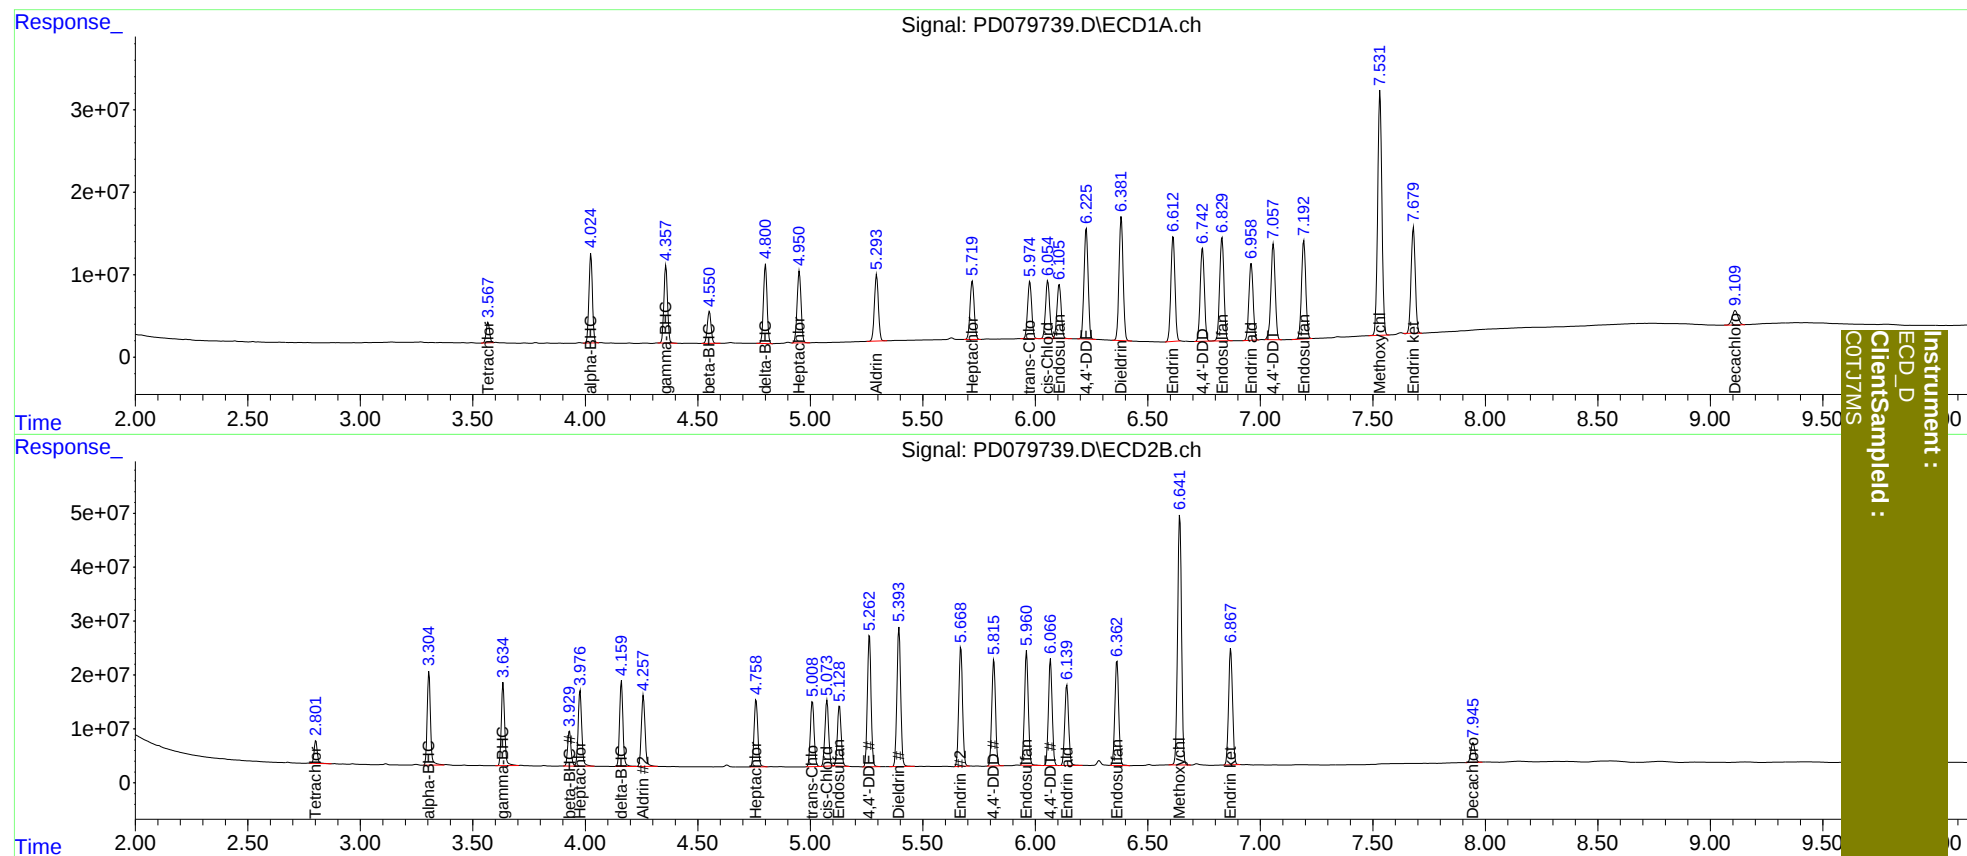

Instrument :
ECD_D
ClientSampled :
COTJMS