

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112024\
 Data File : PD086814.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2024 21:47
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA1010

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 02:42:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 20 02:36:31 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.558	2.885	9747525	65361588	5.355	5.711
27)	SA Decachlor...	9.092	8.091	29830242	146.3E6	11.353	11.522
Target Compounds							
2)	A alpha-BHC	4.008	3.400	16469634	96606674	4.767	5.413
3)	MA gamma-BHC...	4.340	3.737	16825550	90954216	4.922	5.465
4)	MA Heptachlor	4.940	4.093	17254048	97117268	5.054	5.678
9)	A Endosulfan I	6.086	5.260	15086903	81407216	5.134	5.638
13)	MA Dieldrin	6.359	5.525	31681389	169.4E6	9.763	11.110
14)	MA Endrin	6.586	5.802	26193820	155.7E6	9.815	11.298
16)	A 4,4'-DDD	6.717	5.943	22946384	133.6E6	9.789	11.089
17)	MA 4,4'-DDT	7.033	6.198	24022823	142.6E6	9.799	11.034
20)	A Methoxychlor	7.506	6.770	70880111	349.0E6	52.554	60.093


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112024\
Data File : PD086814.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2024 21:47
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 02:42:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 20 02:36:31 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

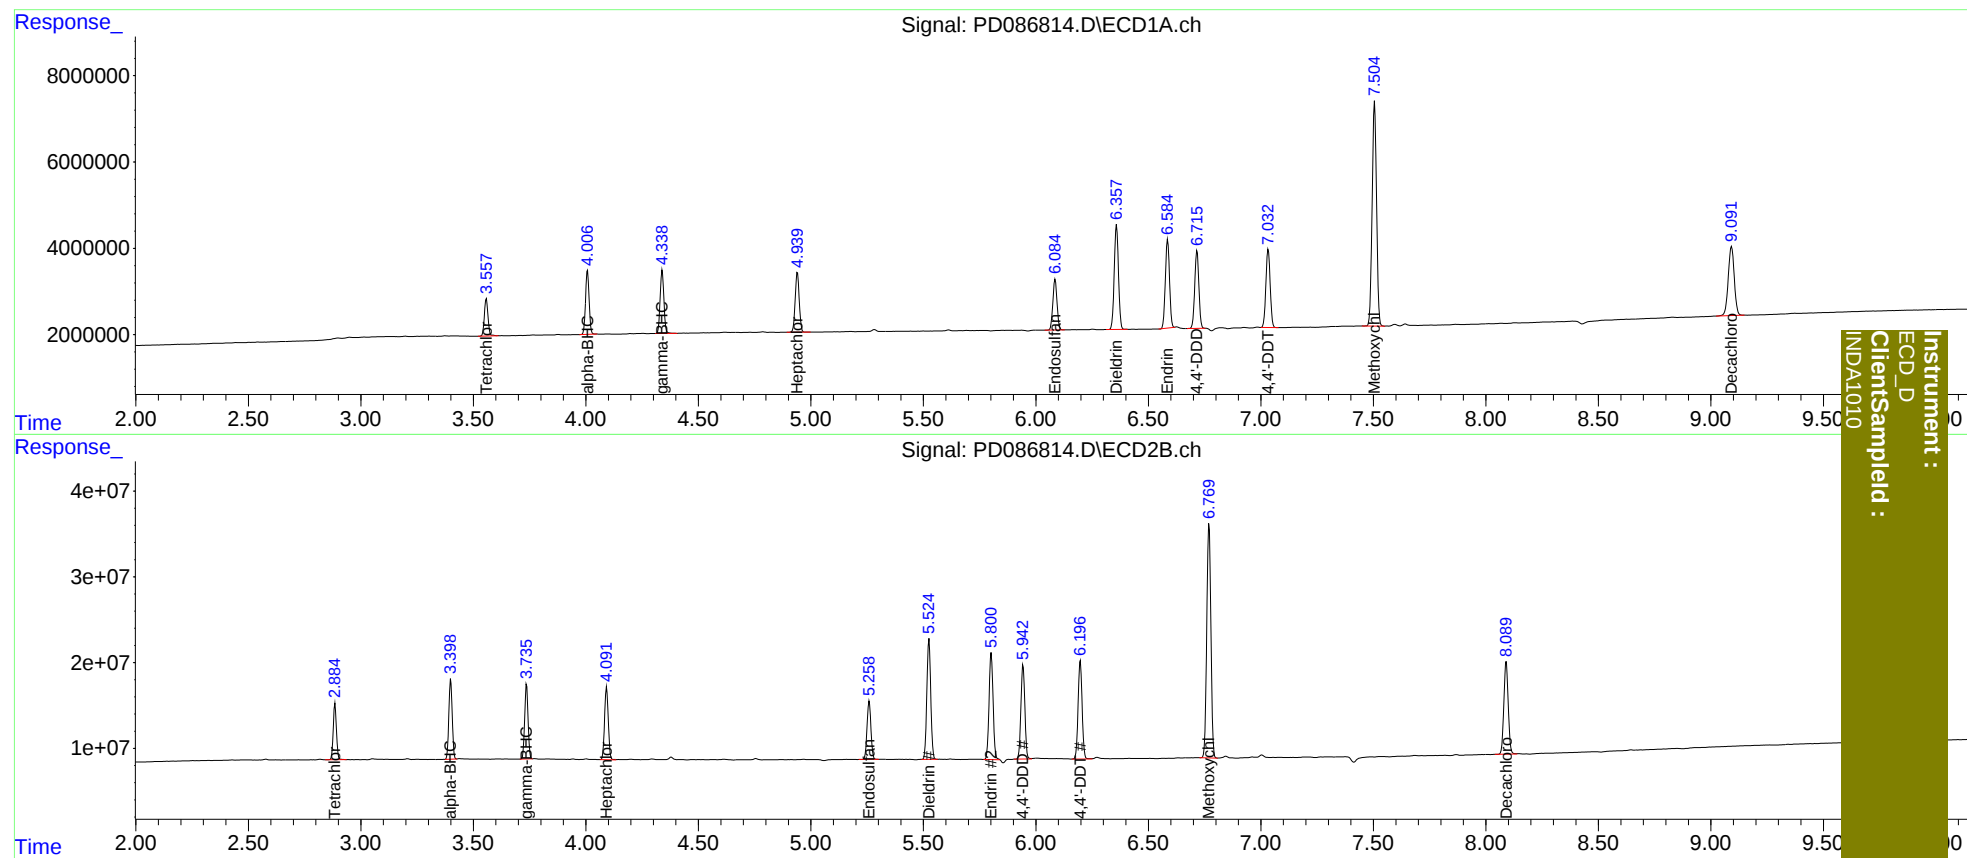


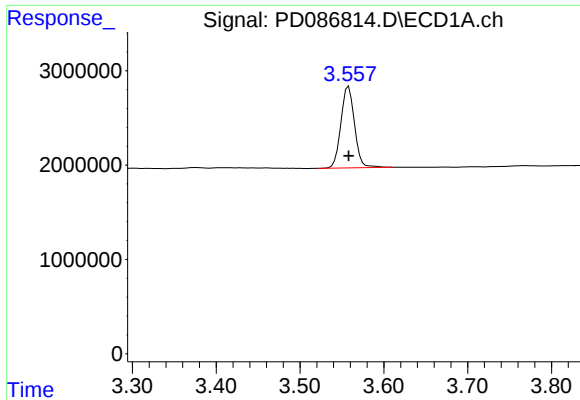

#1 Tetrachloro-m-xylene


R.T.: 3.558 min
Delta R.T.: 0.000 min
Response: 9747525
Conc: 5.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1010

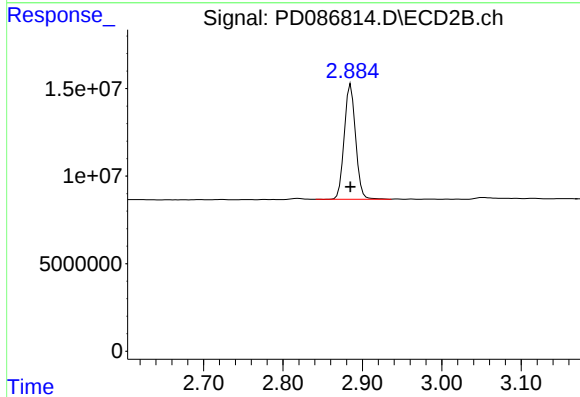


#1 Tetrachloro-m-xylene

R.T.: 2.885 min
Delta R.T.: 0.000 min
Response: 65361588
Conc: 5.71 ng/ml

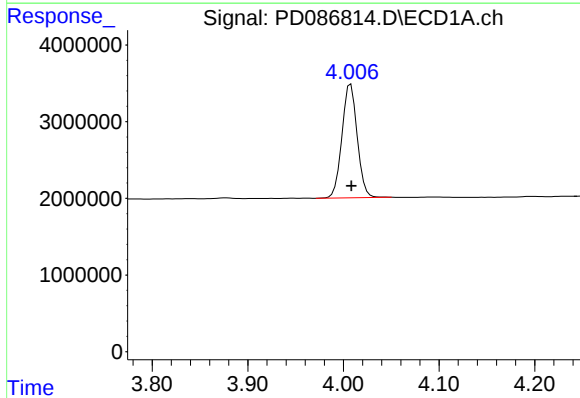


#2 alpha-BHC

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 16469634
Conc: 4.77 ng/ml

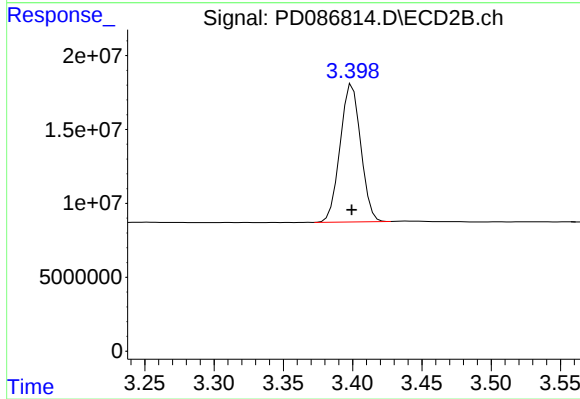

#2 alpha-BHC


R.T.: 3.400 min
Delta R.T.: 0.000 min
Response: 96606674
Conc: 5.41 ng/ml

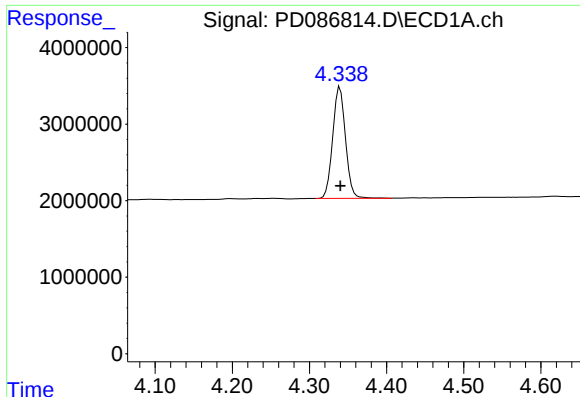

#3 gamma-BHC (Lindane)


R.T.: 4.340 min
Delta R.T.: 0.000 min
Response: 16825550
Conc: 4.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1010

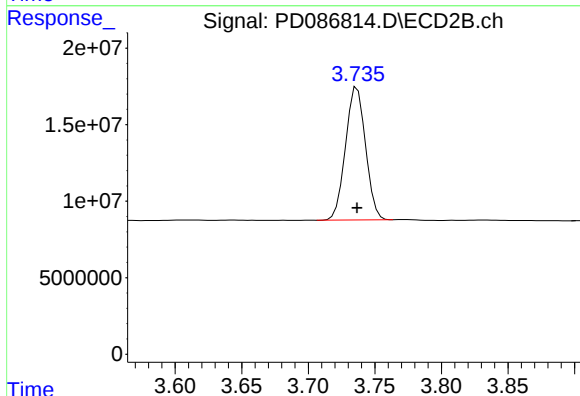


#3 gamma-BHC (Lindane)

R.T.: 3.737 min
Delta R.T.: 0.000 min
Response: 90954216
Conc: 5.46 ng/ml

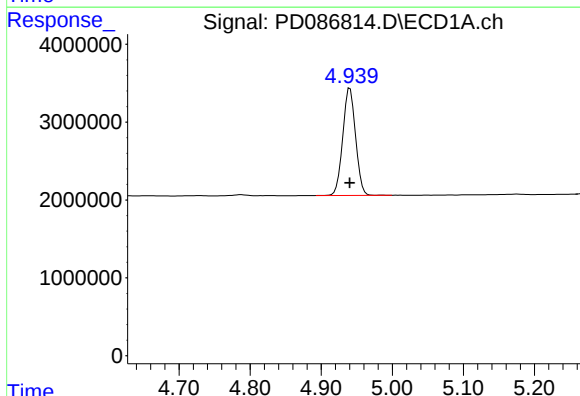


#4 Heptachlor

R.T.: 4.940 min
Delta R.T.: 0.000 min
Response: 17254048
Conc: 5.05 ng/ml

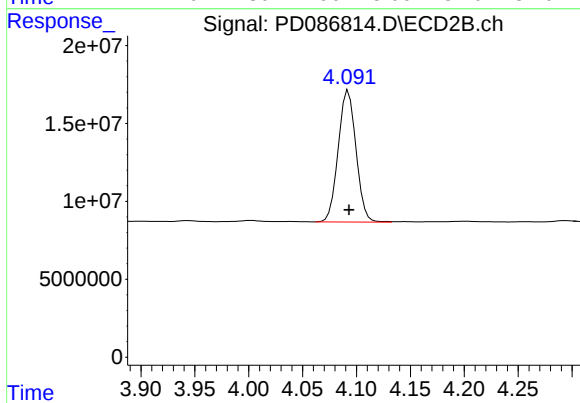

#4 Heptachlor


R.T.: 4.093 min
Delta R.T.: 0.000 min
Response: 97117268
Conc: 5.68 ng/ml

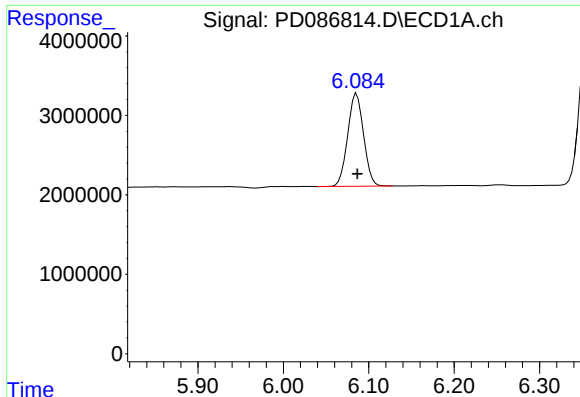

#9 Endosulfan I


R.T.: 6.086 min
Delta R.T.: 0.000 min
Response: 15086903
Conc: 5.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1010

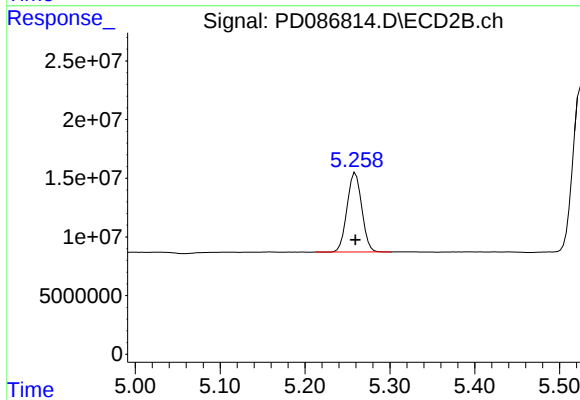


#9 Endosulfan I

R.T.: 5.260 min
Delta R.T.: 0.000 min
Response: 81407216
Conc: 5.64 ng/ml

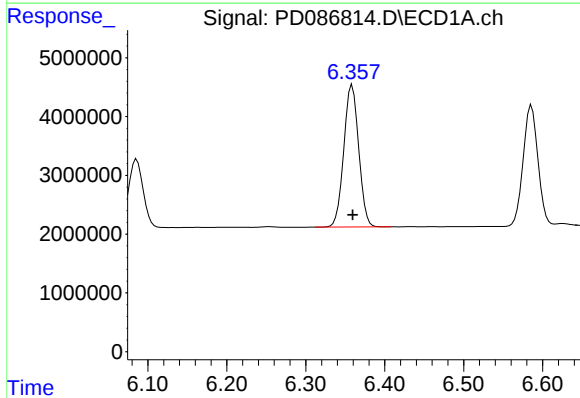


#13 Dieldrin

R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 31681389
Conc: 9.76 ng/ml

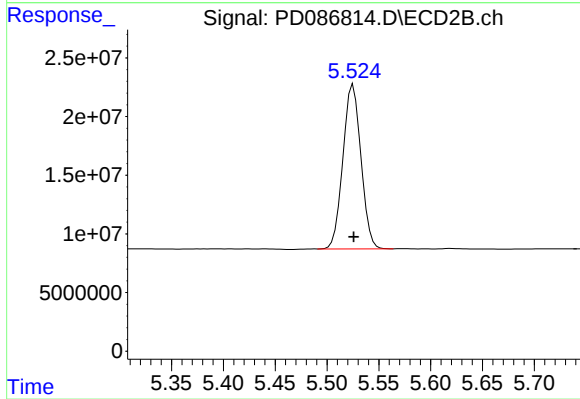

#13 Dieldrin


R.T.: 5.525 min
Delta R.T.: 0.000 min
Response: 169438240
Conc: 11.11 ng/ml

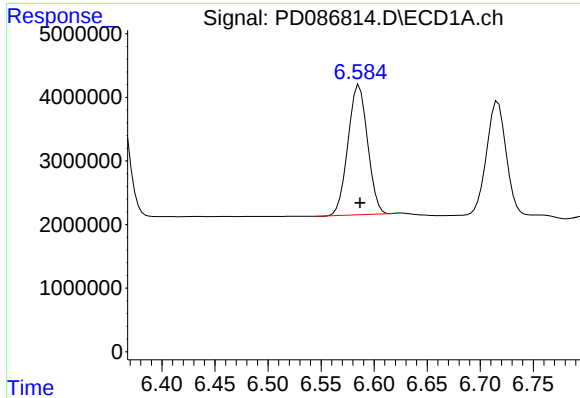

#14 Endrin


R.T.: 6.586 min
Delta R.T.: 0.000 min
Response: 26193820
Conc: 9.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1010

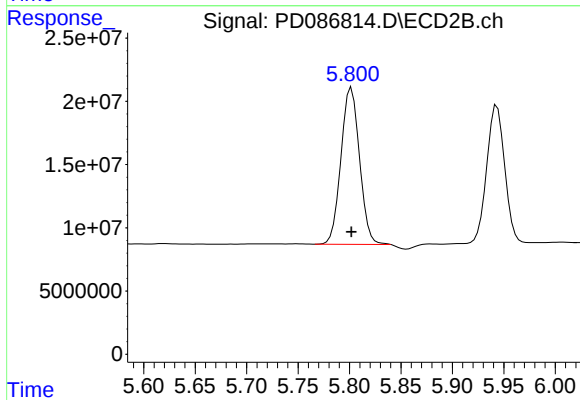


#14 Endrin

R.T.: 5.802 min
Delta R.T.: 0.000 min
Response: 155661302
Conc: 11.30 ng/ml

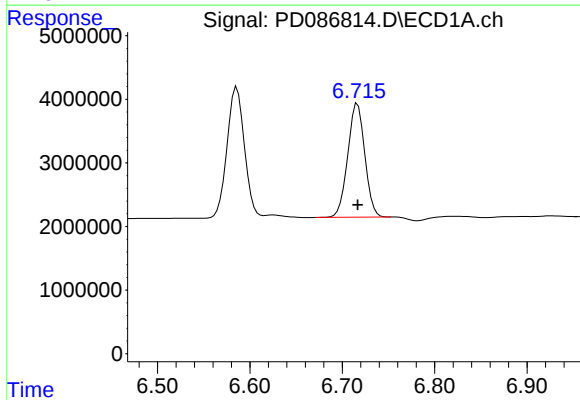


#16 4,4'-DDD

R.T.: 6.717 min
Delta R.T.: 0.000 min
Response: 22946384
Conc: 9.79 ng/ml

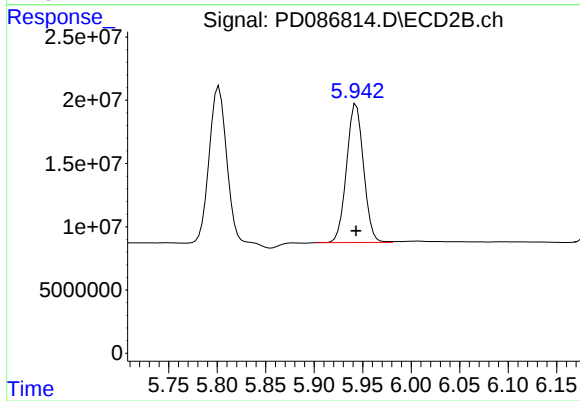

#16 4,4'-DDD


R.T.: 5.943 min
Delta R.T.: 0.000 min
Response: 133557230
Conc: 11.09 ng/ml

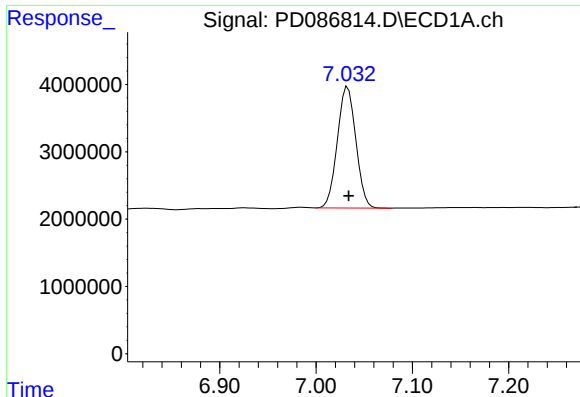

#17 4,4'-DDT


R.T.: 7.033 min
Delta R.T.: 0.000 min
Response: 24022823
Conc: 9.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1010

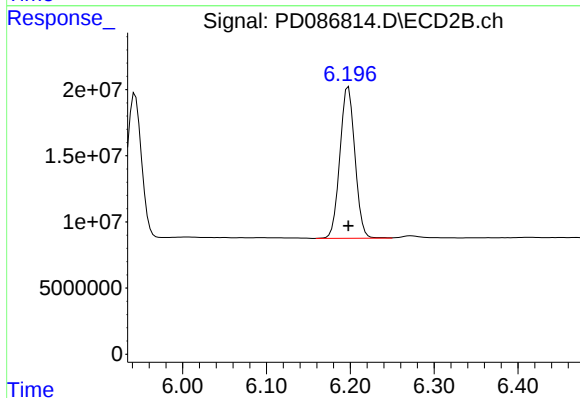


#17 4,4'-DDT

R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 142596057
Conc: 11.03 ng/ml

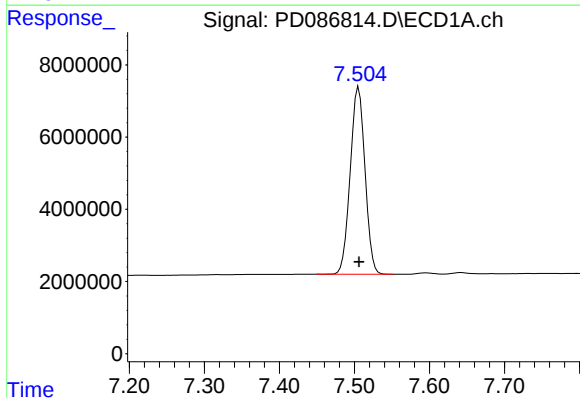


#20 Methoxychlor

R.T.: 7.506 min
Delta R.T.: 0.000 min
Response: 70880111
Conc: 52.55 ng/ml

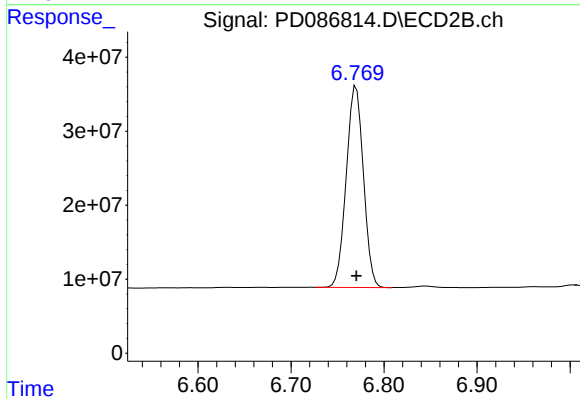

#20 Methoxychlor


R.T.: 6.770 min
Delta R.T.: 0.000 min
Response: 349013865
Conc: 60.09 ng/ml

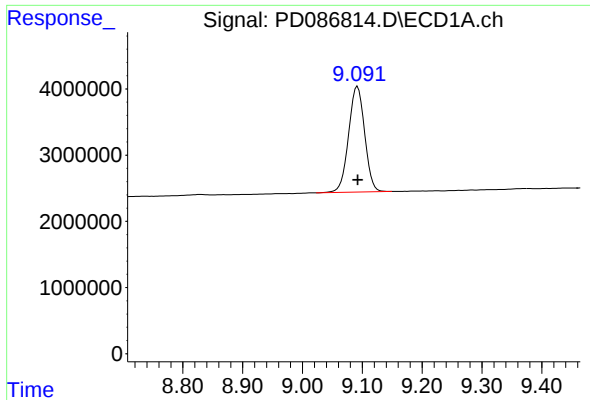

#27 Decachlorobiphenyl

R.T.: 9.092 min
Delta R.T.: 0.000 min
Response: 29830242
Conc: 11.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1010

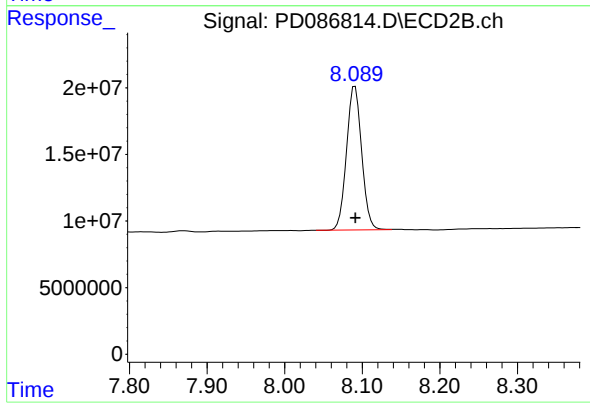

#27 Decachlorobiphenyl

R.T.: 8.091 min
Delta R.T.: 0.000 min
Response: 146298649
Conc: 11.52 ng/ml